


# Technical Information

## Liquiline CM442R/CM444R/ CM448R

Cabinet controller with a maximum of eight measuring channels based on digital Memosens technology

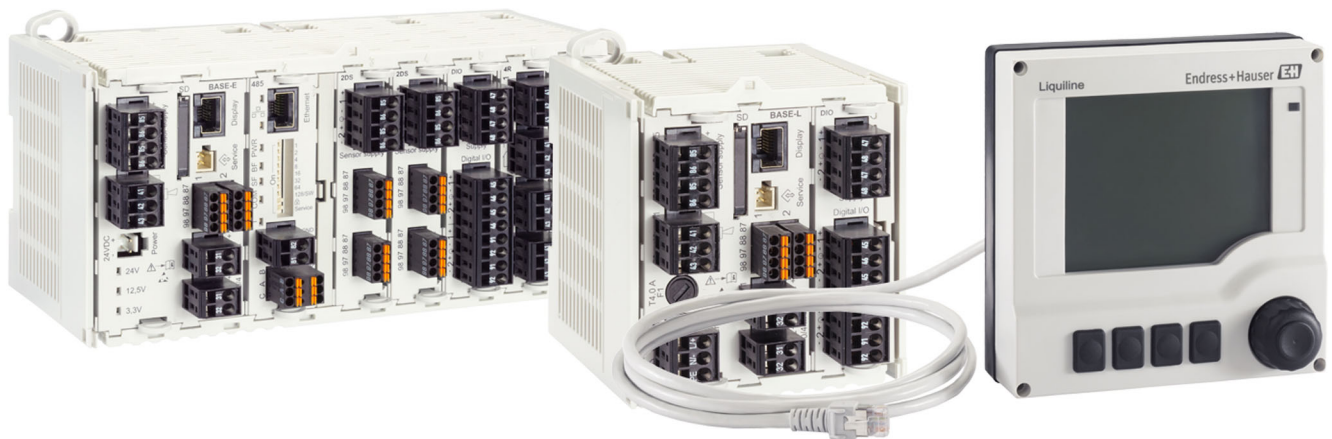

For monitoring and controlling processes in industry and the environmental sector

### Application

- Food and beverages
- Life science
- Water and wastewater
- Chemical industry

### Your benefits

- Highly flexible:
  - Able to connect up to 8 Memosens sensors
  - Mathematics functions calculate new measured values
  - Digital fieldbuses (HART, PROFIBUS, Modbus, Ethernet/IP) and integrated web server
  - Choice of cleaning function, controller and alarm relay
- Optional digital or analog inputs/outputs
- Maximum process safety thanks to standardized operating concept across all devices in the Liquiline, sampler and analyzer platform
- Fast commissioning thanks to:
  - Memosens: lab-calibrated sensors & hot plug-and-play
  - Preconfigured Liquiline transmitter
  - Easy extension and adaptation
- Minimum inventory:
  - Cross-platform, modular concept (e.g. identical modules irrespective of parameters)
  - Integration into Fieldcare and W@M facilitates effective asset management

## Table of contents

<b>Function and system design</b> . . . . .	<b>4</b>	External power supply . . . . .	22
Measuring system . . . . .	4	PFM function . . . . .	22
Application example . . . . .	5	Auxiliary voltage . . . . .	22
		Test voltage . . . . .	22
		Cable specification . . . . .	22
<b>Device architecture</b> . . . . .	<b>6</b>	<b>Current outputs, active</b> . . . . .	<b>22</b>
Slot and port assignment . . . . .	6	Span . . . . .	22
Order of the modules . . . . .	6	Signal characteristic . . . . .	22
Basic rule for hardware upgrades . . . . .	6	Electrical specification . . . . .	22
Determining the hardware delivery status . . . . .	7	Cable specification . . . . .	22
Terminal diagram . . . . .	7	<b>Relay outputs</b> . . . . .	<b>23</b>
Device configuration using the example of a CM442R- **M1A1FO* . . . . .	8	Electrical specification . . . . .	23
Function diagram CM442R . . . . .	9	Cable specification . . . . .	23
Device configuration using the example of a CM444R- **M42A1FA* . . . . .	10	<b>Protocol-specific data</b> . . . . .	<b>23</b>
Function diagram CM444R . . . . .	11	HART . . . . .	23
Device configuration using the example of a CM448R- **26A1* . . . . .	12	PROFIBUS DP . . . . .	24
Function diagram CM448R . . . . .	13	Modbus RS485 . . . . .	24
		Modbus TCP . . . . .	24
<b>Communication and data processing</b> . . . . .	<b>14</b>	EtherNet/IP . . . . .	24
		Web server . . . . .	25
<b>Dependability</b> . . . . .	<b>14</b>	<b>Power supply</b> . . . . .	<b>25</b>
Reliability . . . . .	14	Supply voltage . . . . .	25
Maintainability . . . . .	16	Power consumption . . . . .	25
Safety . . . . .	19	Fuse . . . . .	26
<b>Input</b> . . . . .	<b>20</b>	Overvoltage protection . . . . .	26
Measured variables . . . . .	20	Cable specification for optional display cable . . . . .	26
Measuring ranges . . . . .	20	Electrical connection . . . . .	26
Types of input . . . . .	20	Connecting optional modules . . . . .	28
Input signal . . . . .	20	Protective ground connection . . . . .	29
Cable specification . . . . .	20	Sensor connection . . . . .	30
<b>Digital inputs, passive</b> . . . . .	<b>20</b>	<b>Performance characteristics</b> . . . . .	<b>32</b>
Electrical specification . . . . .	20	Response time . . . . .	32
Span . . . . .	20	Reference temperature . . . . .	32
Nominal input current . . . . .	20	Measured error for sensor inputs . . . . .	32
PFM function . . . . .	20	Measured error for current inputs and outputs . . . . .	32
Test voltage . . . . .	20	Frequency tolerance of digital inputs and outputs . . . . .	32
Cable specification . . . . .	20	Resolution of current inputs and outputs . . . . .	32
<b>Current input, passive</b> . . . . .	<b>20</b>	Repeatability . . . . .	32
Span . . . . .	20	<b>Installation</b> . . . . .	<b>32</b>
Signal characteristic . . . . .	20	Mounting on DIN rail as per IEC 60715 . . . . .	32
Internal resistance . . . . .	20	Wall mounting . . . . .	33
Test voltage . . . . .	20	Mounting the external display . . . . .	34
<b>Output</b> . . . . .	<b>21</b>	<b>Environment</b> . . . . .	<b>34</b>
Output signal . . . . .	21	Ambient temperature range . . . . .	34
Signal on alarm . . . . .	22	Storage temperature . . . . .	35
Load . . . . .	22	Humidity . . . . .	35
Linearization/transmission behavior . . . . .	22	Degree of protection . . . . .	35
		Climate class . . . . .	35
<b>Digital outputs, passive</b> . . . . .	<b>22</b>	Vibration resistance . . . . .	35
Electrical specification . . . . .	22	Electromagnetic compatibility . . . . .	35

Electrical safety . . . . .	36
Degree of contamination . . . . .	36
<b>Mechanical construction . . . . .</b>	<b>36</b>
Dimensions . . . . .	36
Weight . . . . .	39
Materials . . . . .	39
<b>Operability . . . . .</b>	<b>40</b>
External display . . . . .	40
Operating concept . . . . .	40
Local operation via external, optional display . . . . .	40
Remote operation . . . . .	41
Language packages . . . . .	42
<b>Certificates and approvals . . . . .</b>	<b>43</b>
CE mark . . . . .	43
EAC . . . . .	43
cCSAus . . . . .	43
<b>Ordering information . . . . .</b>	<b>43</b>
Product page . . . . .	43
Product Configurator . . . . .	43
Scope of delivery . . . . .	44
<b>Accessories . . . . .</b>	<b>44</b>
Measuring cable . . . . .	44
Sensors . . . . .	44
Additional functionality . . . . .	48
Software . . . . .	50
Other accessories . . . . .	50

## Function and system design


### Measuring system

The overview shows examples of measuring systems. Other sensors and assemblies can be ordered for conditions specific to your application ([www.endress.com/products](http://www.endress.com/products)).

#### Measuring point

A complete measuring system comprises:

- Transmitter Liquiline
- Optional display
- Sensors with Memosens technology
- Assemblies to suit the sensors used

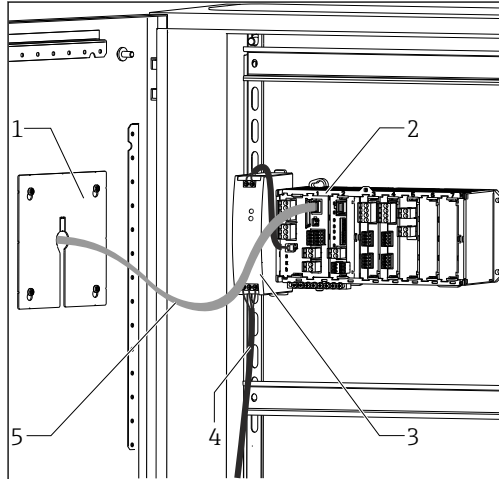


1 Cabinet installation (without sensor and signal cables)

- 1 Optional display (back)
- 2 Liquiline
- 3 External power unit (CM444R and CM448R only)
- 4 Power cable (to be provided by the customer)
- 5 Display cable

#### pH value or ORP

pH measurement in drinking water (→ Fig.)

- Retractable assembly Cleanfit CPA871
- Sensor Orbisint CPS11D
- Measuring cable CYK10



ORP in drinking water

- Dipfit CYA112 immersion assembly
- Sensor Orbisint CPS12D
- Measuring cable CYK10


#### Conductivity

Inductive conductivity measurement in wastewater treatment

- Sensor Indumax CLS50D
- Sensor fixed cable

Conductive conductivity measurement in power plant cooling water


- Sensor Condumax CLS15D
- Measuring cable CYK10



#### Oxygen

Oxygen in aeration basins

- Dipfit CYA112 immersion assembly
- Holder CYH112
- Sensor
  - COS61D (optical) with fixed cable (→ Fig.)
  - COS51D (amperometric), cable CYK10




#### Nitrate and SAC

Nitrate in wastewater

- Sensor CAS51D-\*\*A2 with fixed cable
- Dipfit CYA112 immersion assembly
- Holder CYH112

SAC in the wastewater treatment outlet

- Sensor CAS51D-\*\*2C2 with fixed cable
- Dipfit CYA112 immersion assembly
- Holder CYH112




#### Turbidity and interface

Turbidity in industrial water

- Sensor Turbimax CUS51D with fixed cable (→ Fig.)
- Assembly Flowfit CUA250
- Spray head CUR3 (optional)

Interface in the primary clarifier


- Sensor Turbimax CUS71D
- Assembly CYA112
- Holder CYH112



#### Disinfection

Free available chlorine (and pH) in drinking water


- Sensor CCS142D
- Sensor CPS11D
- Measuring cable CYK10
- Flow assembly CCA250



#### Ion-selective electrodes


Ammonium and nitrate measurement in the aeration basin

- Sensor CAS40D with fixed cable
- Holder CYH112



**Application example**

- Transmitter CM444R-AAM44A0FM6 with:  
4 x Memosens, Modbus TCP, 2 digital inputs and 2 digital outputs, 2 x relays for cleaning/limit value, 2 x analog current input
- pH and temperature with CPS11D, item 1 (www.endress.com/cps11d)
- Chlorine with CCS142D, item 4 (www.endress.com/ccs142d)
- 2 x conductivity, inductive measurement with CLS50D, item 2 and 3 (www.endress.com/cls50d)
- 1 x measuring range switching for conductivity via Modbus module
- Flow assembly CCA250 with optional proximity switch INS (www.endress.com/caa250)
- Chlorine regulation with dosing interrupted if no flow: proximity switch via digital input of DIO module, flow feedforward control (via digital or analog input), PFM-controlled dosing pump via digital output of DIO module

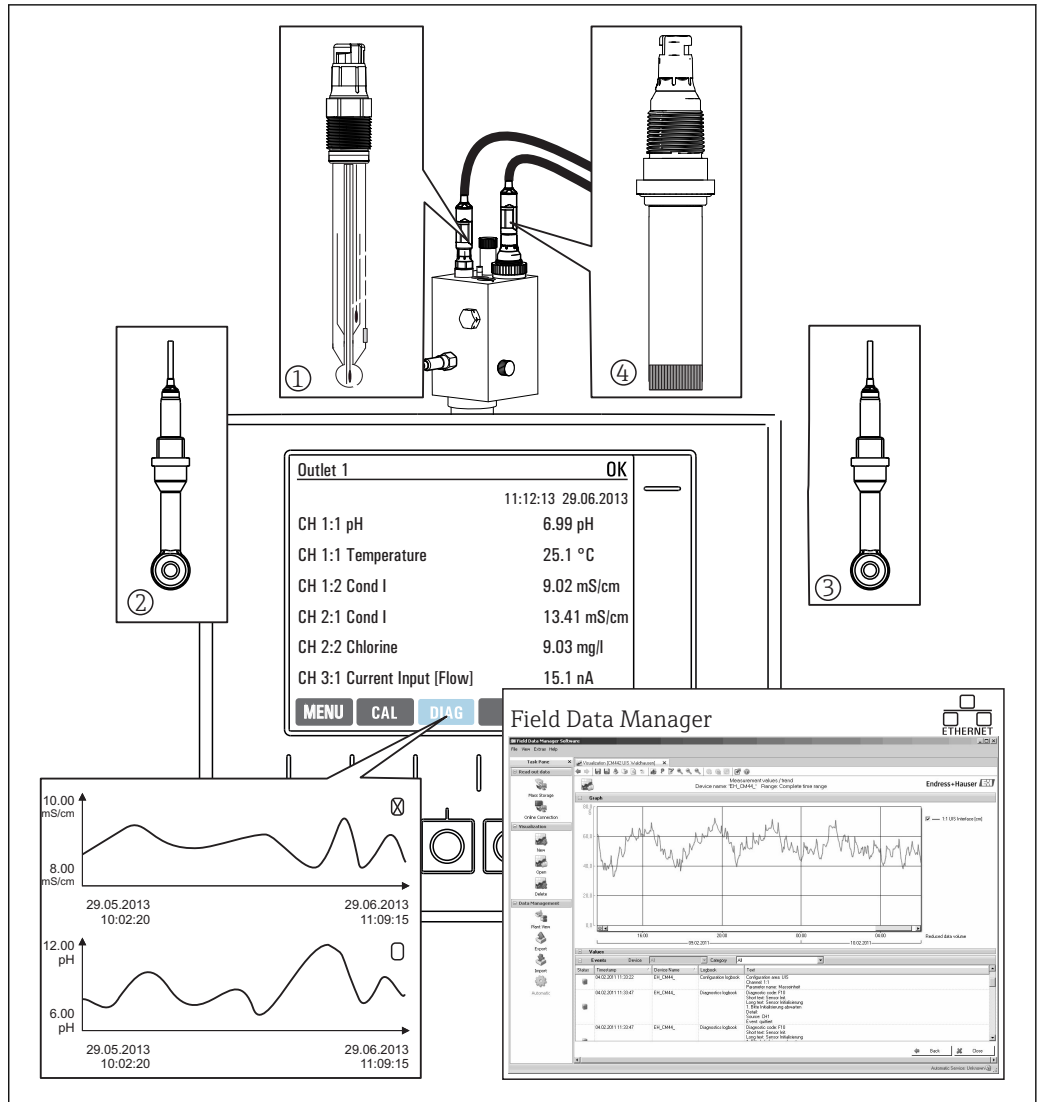

A0025347



2 Measuring point in the CIP process

**Data retention**

- Storage of all measured values, incl. values of external sources, in the non-volatile memory (data logbook)
- Data called up on site via user-defined measuring menu and load curve display of the data logbook
- Transmission of data by ethernet, CDI interface or SD card and storage in a tamper-proof database (Field Data Manager)
- Data export to csv file (for Microsoft Excel)

## Device architecture

### Slot and port assignment

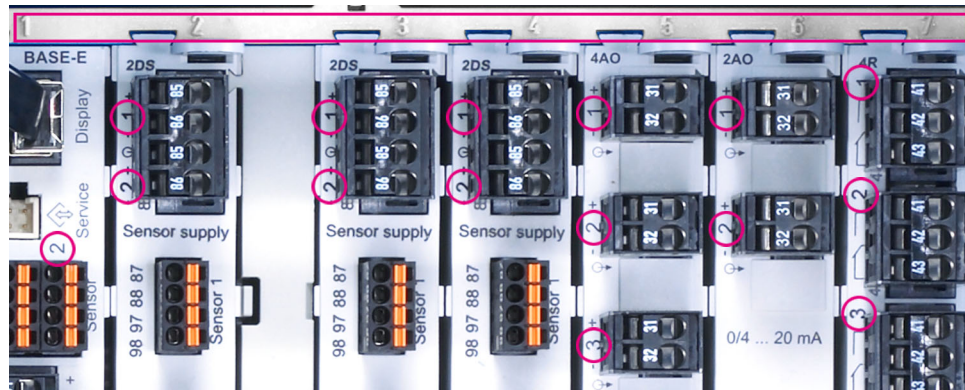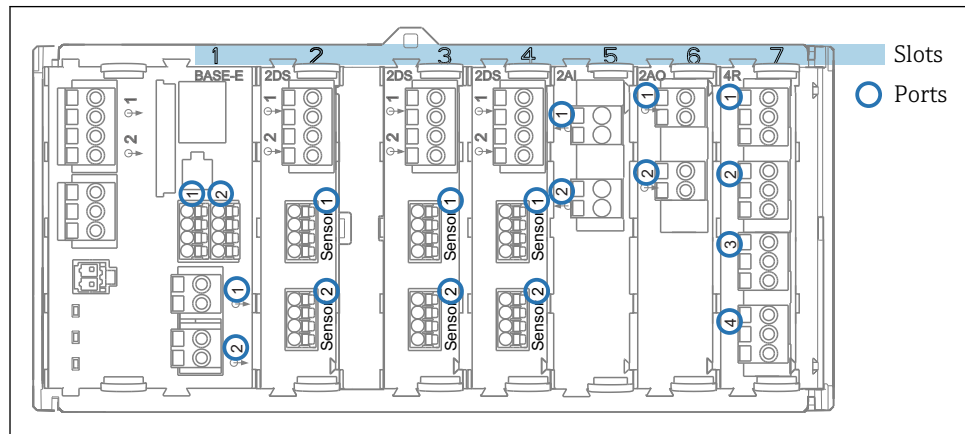

3 Slot and port assignment of the hardware modules

Outlet 1	OK	Port Slot
CH1: 1:1 pH Glass	ATC 6.95 pH	
CH2: 1:2 TU/TS	500.0 g/l	
CH3: 5:1 SAC	500.0 1/m	
CH4: 5:2 Cond i	ATC 2.62 mS/cm	
CH5: 6:1 Chlorine	28.33 mg/l	
CH6: 6:2 Redox	± 51 mV	
CH7: 7:1 Oxygen (am...)	32.86 mg/l	
CH8: 7:2 Cond c	ATC 131.1 µS/cm	

4 Slot and port assignment on the display

- Inputs are assigned to measuring channels in the ascending order of the slots and ports. Adjacent example: "CH1: 1:1 pH glass" means: Channel 1 (CH1) is slot 1 (basic module) : Port 1 (input 1), pH glass sensor
- Outputs and relays are named according to their function, e.g. "current output", and are displayed with the slot and port numbers in ascending order

### Order of the modules

Depending on the version ordered, the device is supplied with a number of electronic modules, which are assigned in a specific sequence in ascending order to slots 0 to 7. If you do not have a particular module, the next moves up automatically:

- The basic module (which is always present) always occupies slots 0 and 1
- Fieldbus module 485 or Ethernet module ETH (only one of the two modules can be used)
- Memosens input module 2DS (DS = digital sensor)
- Extension module for digital inputs and outputs DIO (DIO = digital input and output)
- Current input module 2AI (AI = analog input)
- Current output module 4AO or 2AO (AO = analog output)
- Relay modules AOR, 4R or 2R (AOR = analog output + relay, R = relay)

**i** Modules with 4 ports are connected before modules of the same type with 2 ports.

### Basic rule for hardware upgrades

- i** Please note the following if upgrading the device:
- The sum of all current inputs and outputs may not exceed 8!
  - A maximum of two "DIO" modules may be used.

**Determining the hardware delivery status**


You must be aware of the type of modules and the number of them supplied with the device you have ordered to determine the delivery status of your Liquiline.

- Basic module  
One basic module in all versions. Always occupies slots 0 and 1.
- Fieldbus module  
Optional, and only one fieldbus module is possible.
- Input modules
  - Must be clearly assigned to the number of optional inputs ordered.
  - Examples:
    - 2 current inputs = module 2AI
    - 4 Memosens inputs = 2 inputs with basic module + module 2DS with 2 further inputs
- Current outputs and relays  
Various module combinations can exist.  
The following table will help you determine which modules your device has, depending on the type and number of outputs.

Current outputs	Relays		
	0	2	4
2	-	1 x 2R	1 x 4R
4	1 x 2AO	1 x AOR	1 x 2AO + 1 x 4R
6	1 x 4AO	1 x 4AO + 1 x 2R	1 x 4AO + 1 x 4R
8	1 x 4AO + 1 x 2AO	1 x 4AO + 1 x 2AO + 1 x 2R	1 x 4AO + 1 x 2AO + 1 x 4R

- ▶ Sum up the number of modules and sort them according to the specified sequence → 6.
- ↳ This will give you the slot assignment for your device.


**Terminal diagram**


 The unique terminal name is derived from:  
Slot no. : Port no. : Terminal

**Example, NO contact of a relay**


Device with 4 inputs for digital sensors, 4 current outputs and 4 relays

- Base module BASE-E (contains 2 sensor inputs, 2 current outputs)
- 2DS module (2 sensor inputs)
- 2AO module (2 current outputs)
- 4R module (4 relays)

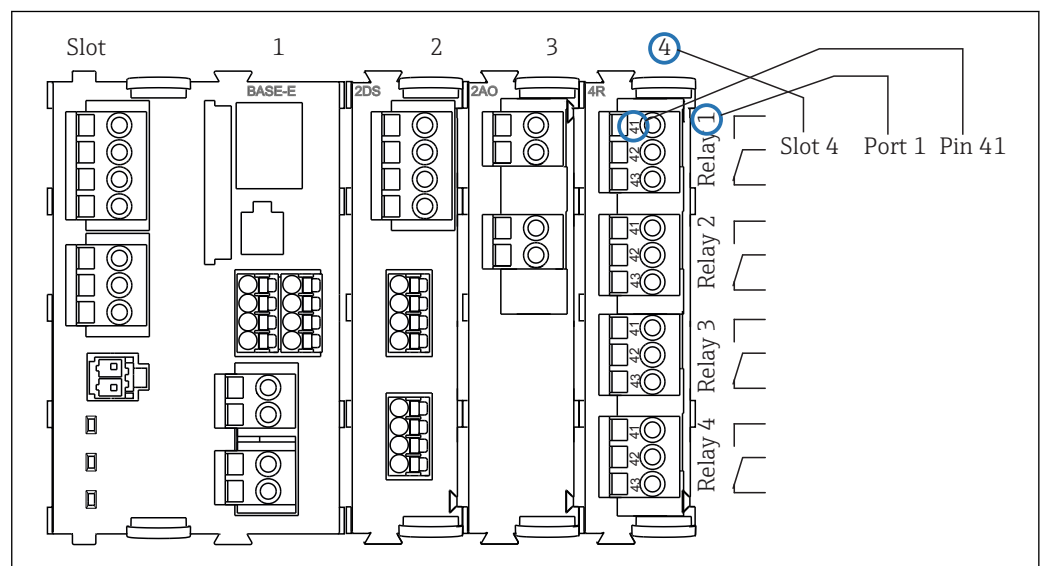

 5 Creating a terminal diagram using the example of the NO contact (terminal 41) of a relay

Device configuration using  
the example of a CM442R-  
\*\*M1A1F0\*

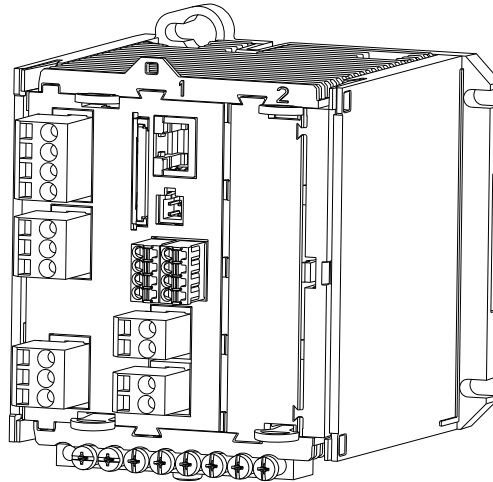


A0025348

<b>Ordered basic device (example)</b>	<ul style="list-style-type: none"> <li>▪ Order code CM442R-**M1A1F0*</li> <li>▪ Functionality: 1 x Memosens, 2 current outputs without HART</li> </ul>
<b>Extension options without additional modules</b>	<ul style="list-style-type: none"> <li>▪ Second Memosens input (71114663)</li> <li>▪ HART with activation code (71128428)</li> </ul>
<b>Extension options by using an extension module in free slot 2</b>	<ul style="list-style-type: none"> <li>▪ Ethernet/PROFIBUS DP/Modbus with module 485 incl. activation code for the desired communication protocol: <ul style="list-style-type: none"> <li>- PROFIBUS DP (71140888)</li> <li>- Modbus RS485 (71140889)</li> <li>- Modbus TCP (71140890)</li> <li>- EtherNet/IP (71219868)</li> <li>- Only Ethernet without fieldbus (71135634)</li> </ul> </li> <li>▪ Alternative for Ethernet or Modbus TCP: module ETH</li> </ul> <p><b>i</b> If you retrofit module 485, any existing current outputs are disabled! Alternative: ETH (Ethernet, Modbus TCP only).</p> <p>Additional inputs or outputs, relays:</p> <ul style="list-style-type: none"> <li>- Module 2AI (71135639): 2 current inputs</li> <li>- Module 2AO (71135632): 2 current outputs</li> <li>- Module AOR (71111053): 2 current outputs, 2 relays</li> <li>- Module 2R (71125375) or 4R (71125376): 2 or 4 relays</li> <li>- Module DIO (71135638): 2 digital inputs and 2 digital outputs</li> </ul>
<b>Basic rule for extensions</b>	The sum of all current inputs and outputs may not exceed 8!
<b>Restrictions if using CUS71D sensors for interface measurement</b>	Only one CUS71D can be connected. The second Memosens input may not be used.
<b>Product Configurator</b>	<a href="http://www.endress.com/cm442r">www.endress.com/cm442r</a>



Function diagram CM442R

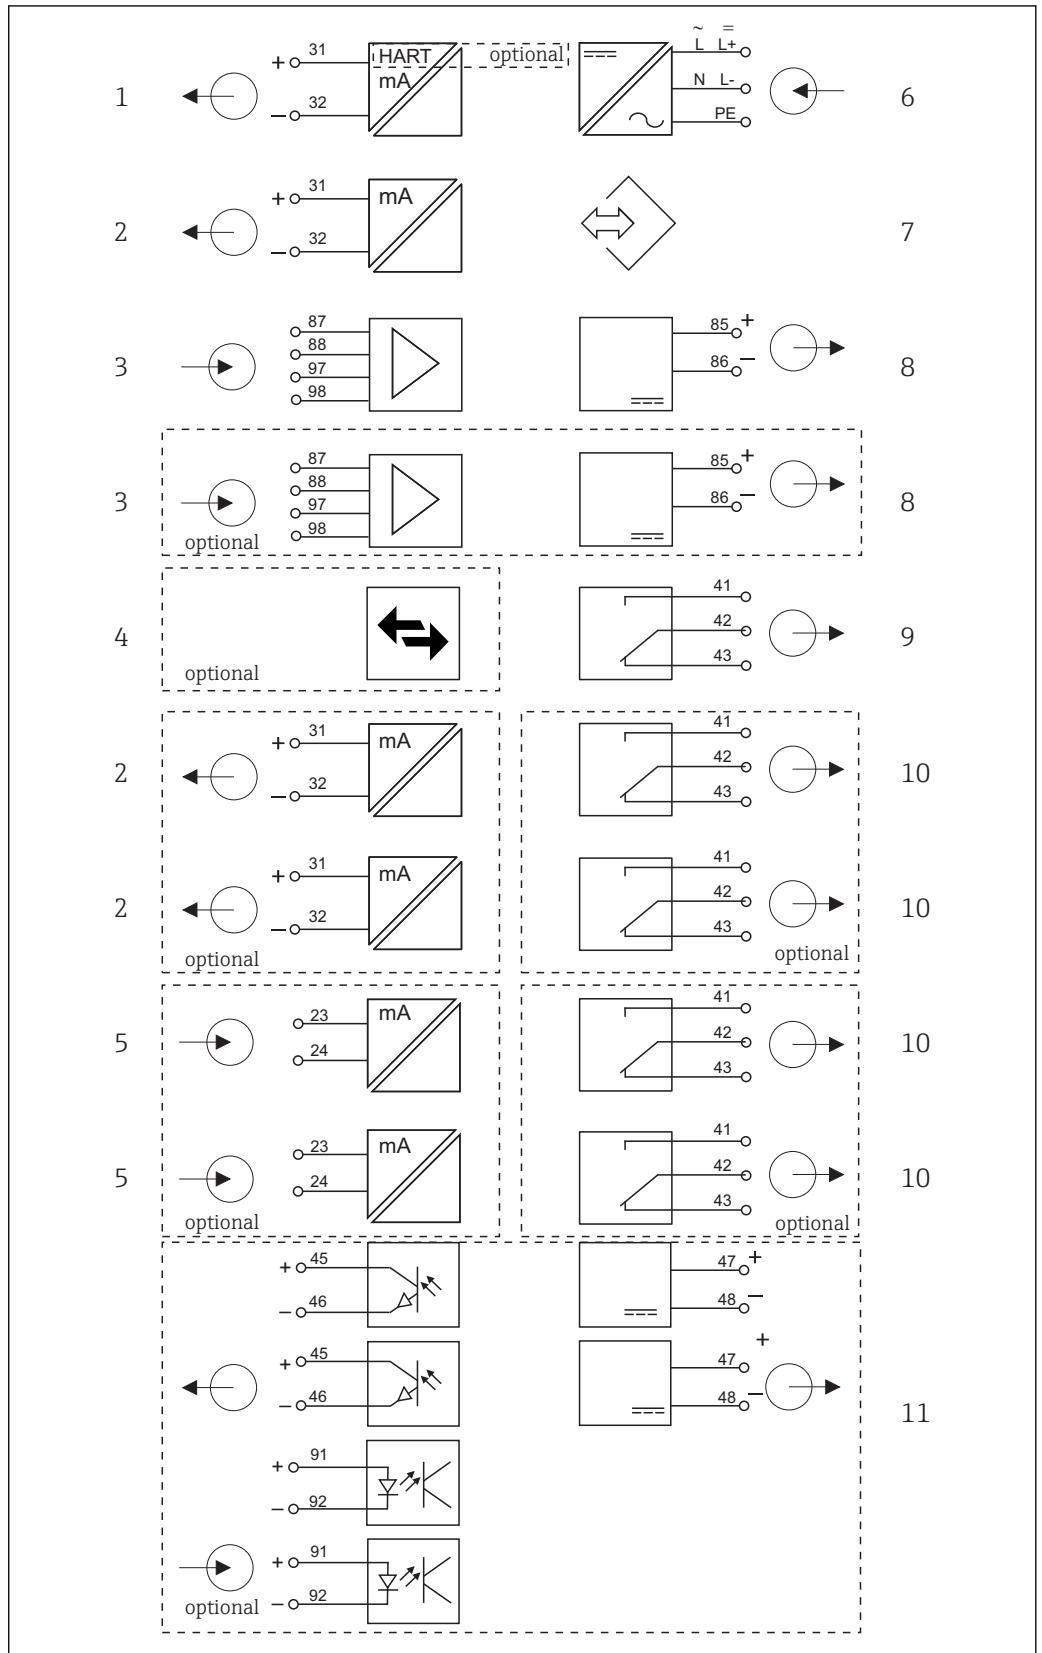


A0015791

6 Block circuit diagram CM442R


- |   |  |    |   |
|---|--|----|---|
| 1 | Current output 1:1, + HART (optional)  | 6  | Power connection                        |
| 2 | Current outputs (2 x optional)         | 7  | Service interface                       |
| 3 | 2 x Memosens input (1 x optional)      | 8  | Power supply, fixed cable sensors       |
| 4 | PROFIBUS DP/Modbus/Ethernet (optional) | 9  | Alarm relay                             |
| 5 | 2 x current input (optional)           | 10 | 2 or 4 x relays (optional)              |
|   |  | 11 | 2 digital inputs and outputs (optional) |

Device configuration using the example of a CM444R-**\*\*M42A1FA\***

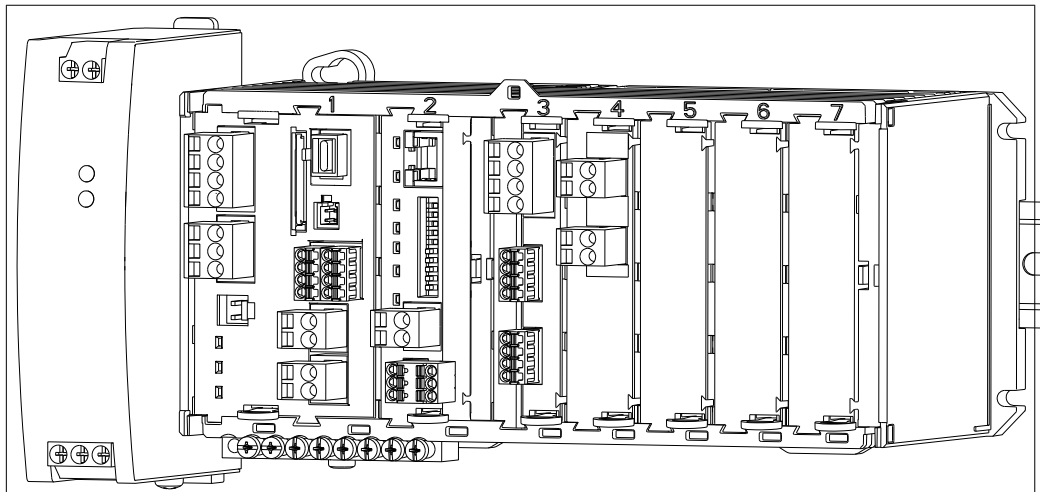

<p><b>Ordered basic device (example)</b></p>	<ul style="list-style-type: none"> <li>▪ Order code CM444R-<b>**M42A1FA*</b></li> <li>▪ Functionality:                         <ul style="list-style-type: none"> <li>- 4 x Memosens (2 on BASE-E module + 2 on an extension module 2DS)</li> <li>- PROFIBUS communication (module 485)</li> <li>- 2 current outputs without HART (on BASE-E module)</li> <li>- 2 current inputs (module 2AI)</li> </ul> </li> </ul> <p>3 slots are still free in this example. More or fewer slots can be free in other versions.</p>
<p><b>Extension options without additional modules</b></p>	<p>None</p>
<p><b>Modification options without additional modules</b></p>	<ul style="list-style-type: none"> <li>▪ Communication type changed by entering activation code. This disables the communication type used previously!                         <ul style="list-style-type: none"> <li>- Modbus RS485 (71140889)</li> <li>- Modbus TCP (71140890)</li> <li>- EtherNet/IP (71219868)</li> </ul> </li> <li>▪ Retrofit to HART by removing module 485 and entering activation code for HART (71128428)</li> </ul>
<p><b>Extension options by using extension modules in free slots 5-7</b></p>	<p>Only the following is possible for the example above: Module 2R (71125375) or 4R (71125376): 2 or 4 relays</p> <p>If extending to eight measuring channels:</p> <ul style="list-style-type: none"> <li>▪ Module 2DS (71135631): 2 Memosens inputs</li> <li>▪ Use of the 2 current outputs in the basic module by entering activation code (71140891)</li> </ul> <p>Additional inputs or outputs and relays if fieldbus module 485 is removed:</p> <ul style="list-style-type: none"> <li>▪ Module 2AO (71135632): 2 current outputs</li> <li>▪ Module AOR (71111053): 2 current outputs, 2 relays</li> <li>▪ Module 2R (71125375) or 4R (71125376): 2 or 4 relays</li> <li>▪ Module DIO (71135638): 2 digital inputs and 2 digital outputs</li> </ul> <p><b>i</b> If you replace module 485 with ETH, you can operate up to 6 current outputs in addition to the ETH module's ethernet or Modbus function. Only two current outputs are possible with 485.</p>
<p><b>Basic rule for extensions</b></p>	<p>The sum of all current inputs and outputs may not exceed 8!</p>
<p><b>Restrictions if using CUS71D sensors for interface measurement</b></p>	<ul style="list-style-type: none"> <li>▪ With the CM444R, any combination of maximum 4 Memosens sensors is possible.</li> <li>▪ An extension to CM448R is not advisable as the maximum number of Memosens inputs remains limited to 4 if a CUS71D is used.</li> </ul>
<p><b>Product Configurator</b></p>	<p><a href="http://www.endress.com/cm444r">www.endress.com/cm444r</a></p>

Function diagram CM444R

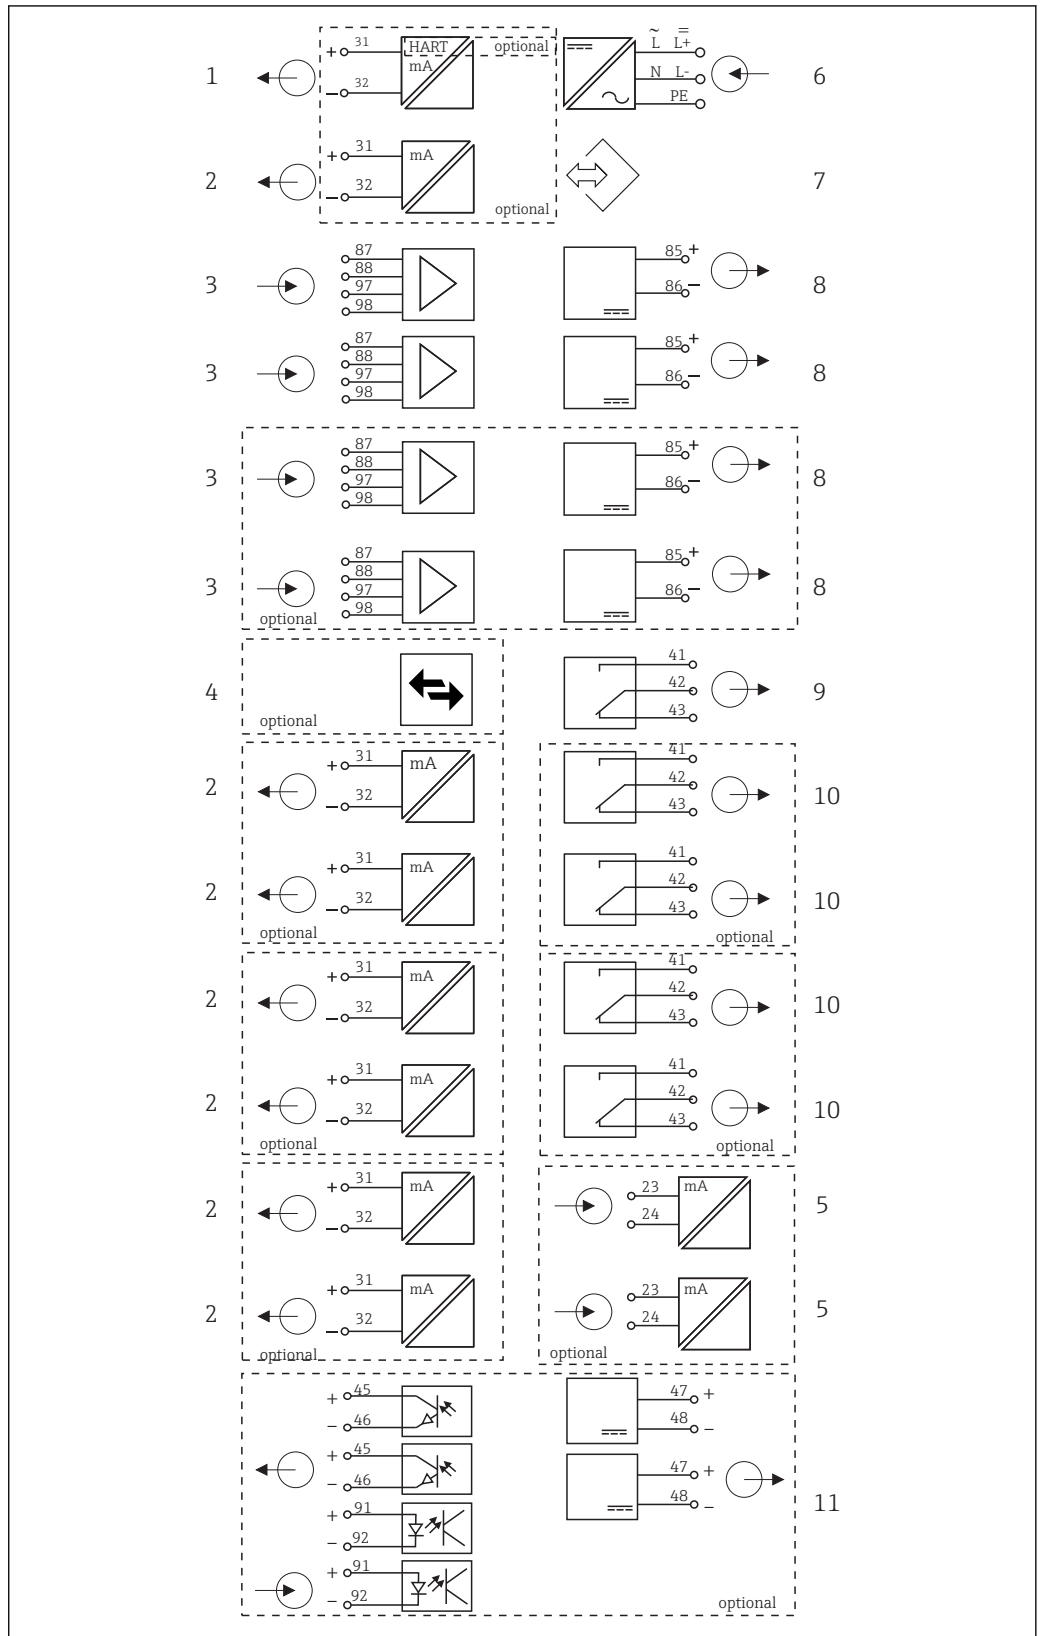


A0015827

7 Block circuit diagram CM444R


- |   |  |    |   |
|---|--|----|---|
| 1 | Current output 1:1, + HART (both optional)   | 6  | Power connection                        |
| 2 | Max. 7 x current output (optional)           | 7  | Service interface                       |
| 3 | Memosens input (2 x standard + 2 x optional) | 8  | Power supply, fixed cable sensors       |
| 4 | PROFIBUS DP/Modbus/Ethernet (optional)       | 9  | Alarm relay                             |
| 5 | 2 x current input (optional)                 | 10 | 2 or 4 x relays (optional)              |
|   |  | 11 | 2 digital inputs and outputs (optional) |

Device configuration using the example of a CM448R-\*\*26A1\*

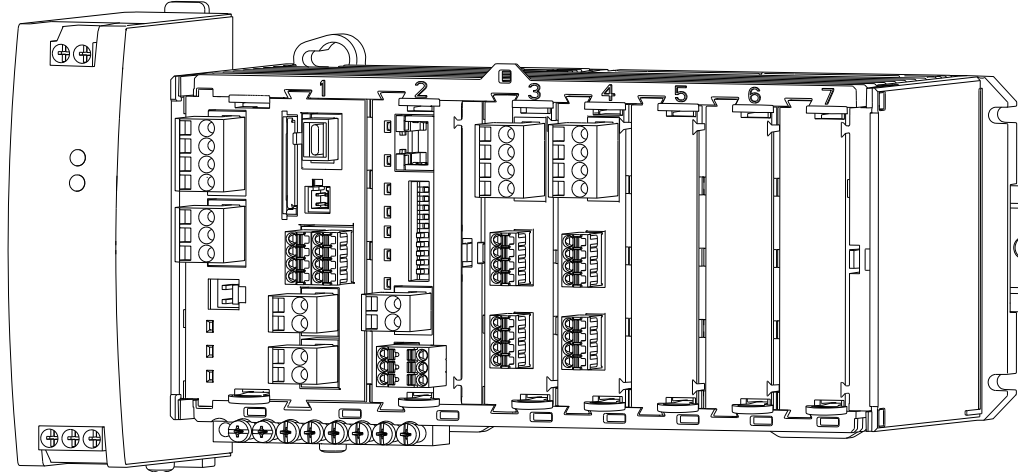

<p><b>Ordered basic device (example)</b></p>	<ul style="list-style-type: none"> <li>▪ Order code CM448R-**26A1*</li> <li>▪ Functionality:                             <ul style="list-style-type: none"> <li>- 6 x Memosens (2 on BASE-E module + 2 on two extension modules 2DS)</li> <li>- PROFIBUS communication (module 485)</li> </ul> </li> </ul> <p>3 slots are still free in this example. More or fewer slots can be free in other versions.</p>
<p><b>Extension options without additional modules</b></p>	<p>None</p>
<p><b>Modification options without additional modules</b></p>	<ul style="list-style-type: none"> <li>▪ Communication type changed by entering activation code. This disables the communication type used previously!                             <ul style="list-style-type: none"> <li>- Modbus RS485 (71140889)</li> <li>- Modbus TCP (71140890)</li> <li>- EtherNet/IP (71219868)</li> </ul> </li> <li>▪ Retrofit to HART by removing module 485 and entering activation code for HART (71128428)</li> </ul>
<p><b>Extension options by using extension modules in free slots 5-7</b></p>	<p>Only the following is possible for the example above: Module 2R (71125375) or 4R (71125376): 2 or 4 relays</p> <p>If extending to eight measuring channels:</p> <ul style="list-style-type: none"> <li>▪ Module 2DS (71135631): 2 Memosens inputs</li> <li>▪ Use of the 2 current outputs in the basic module by entering activation code (71140891)</li> </ul> <p>Additional inputs or outputs, relays:</p> <ul style="list-style-type: none"> <li>▪ Module 2AO (71135632): 2 current outputs</li> <li>▪ Module 2AI (71135639): 2 current inputs</li> <li>▪ Module AOR (71111053): 2 current outputs, 2 relays</li> <li>▪ Module 2R (71125375) or 4R (71125376): 2 or 4 relays</li> <li>▪ Module DIO (71135638): 2 digital inputs and 2 digital outputs</li> </ul> <p><b>i</b> If you replace module 485 with ETH, you can operate up to 6 current outputs in addition to the ETH module's ethernet or Modbus function. Only two current outputs are possible with 485.</p>
<p><b>Basic rule for extensions</b></p>	<p>The sum of all current inputs and outputs may not exceed 8!</p>
<p><b>Restrictions if using CUS71D sensors for interface measurement</b></p>	<p>The maximum number of Memosens inputs that can be used is limited to 4! Here, every combination of CUS71D and other Memosens sensors is then possible.</p>
<p><b>Product Configurator</b></p>	<p><a href="http://www.endress.com/cm448r">www.endress.com/cm448r</a></p>

Function diagram CM448R

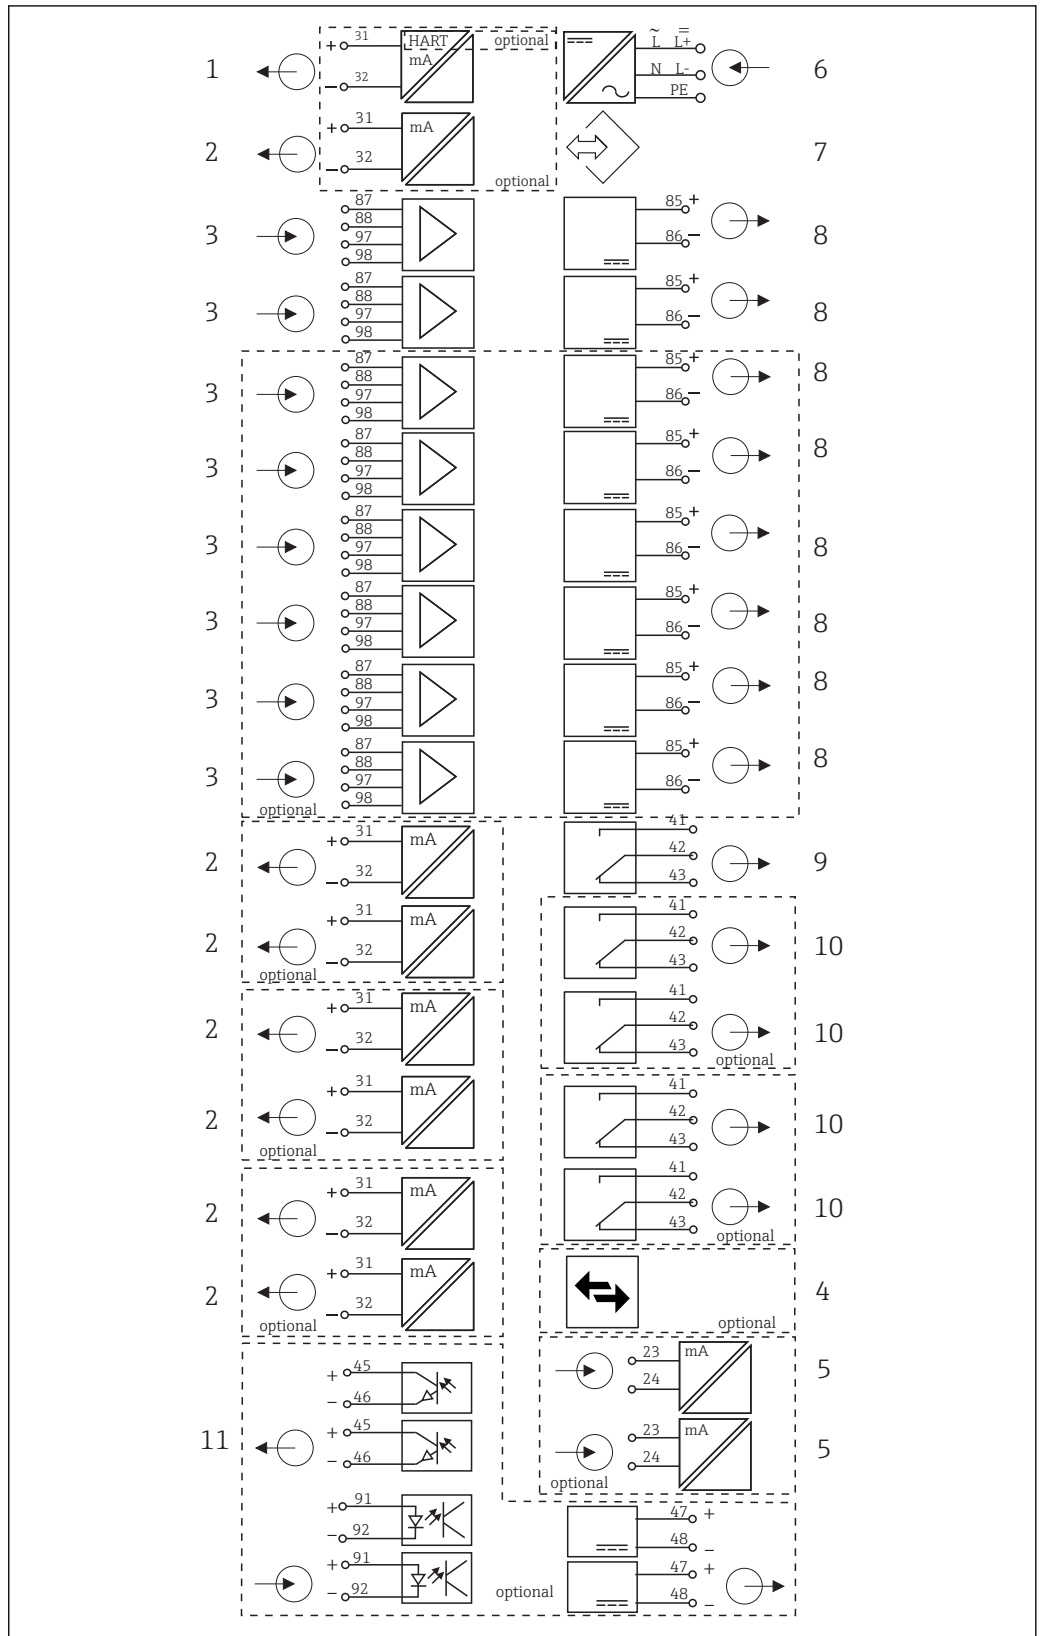

A0015828


8 Function diagram CM448R

- |   |  |    |   |
|---|--|----|---|
| 1 | Current output 1:1, + HART (both optional)         | 7  | Service interface                       |
| 2 | Max. 7 x current output (optional)                 | 8  | Power supply, fixed cable sensors       |
| 3 | Max 8 x Memosens input (2 x of which are optional) | 9  | Alarm relay                             |
| 4 | PROFIBUS DP/Modbus/Ethernet (optional)             | 10 | 2 or 4 x relays (optional)              |
| 5 | 2 x current input (optional)                       | 11 | 2 digital inputs and outputs (optional) |
| 6 | Power connection                                   |    |   |

## Communication and data processing

### Types of communication:

- Fieldbuses
  - HART
  - PROFIBUS DP (Profile 3.02)
  - Modbus TCP or RS485
- EtherNet/IP

 Only one type of Fieldbus communication can ever be active. The last activation code entered decides which bus is used.

The device drivers available make it possible to perform a basic setup and display measured values and diagnostics information via the fieldbus. A full device configuration via the fieldbus is not possible.

### Extension module 485 and current outputs

For PROFIBUS DP, Modbus and Ethernet communication protocols:

- CM442R
  - Current outputs cannot be used in parallel. Any existing current outputs are deactivated with the installation of 485.
- CM444R/CM448R
  - A maximum of 2 current outputs can be used in parallel.

### Extension module ETH and current outputs

- Communication via Ethernet or EtherNet/IP
- CM442R
  - A maximum of 2 current outputs can be used in parallel.
- CM444R and CM448R
  - A maximum of 6 current outputs can be used in parallel.

### Bus termination on the device

- Via slide switch at bus module 485
- Displayed via LED "T" on bus module 485

## Dependability

### Reliability

#### Memosens

Memosens makes your measuring point safer and more reliable:

- Non-contact, digital signal transmission enables optimum galvanic isolation
- No contact corrosion
- Completely watertight
- Sensor can be calibrated in a lab, thus increasing the availability of the measuring point in the process
- Intrinsically safe electronics mean operation in hazardous areas is not a problem.
- Predictive maintenance thanks to recording of sensor data, e.g.:
  - Total hours of operation
  - Hours of operation with very high or very low measured values
  - Hours of operation at high temperatures
  - Number of steam sterilizations
  - Sensor condition

#### Heartbeat diagnostics

- Heartbeat diagnostics screen with graphic indicators for the health of the device and sensor and with a maintenance or (sensor-dependent) calibration timer
- Heartbeat status information on the health of the device and the condition of the sensor
  - 😊: Sensor/device condition or maintenance timer > 20 %; no action is required
  - 😐: Sensor/device condition or maintenance timer > 5 ≤ 20 %, maintenance not yet urgent but should be scheduled
  - ☹️: Sensor/device condition or maintenance timer < 5 %, maintenance is recommended
- The Heartbeat sensor condition is the assessment of the calibration results and the sensor diagnostic functions.

An unhappy smiley can be due to the calibration result, the measured value status or to the operating hours limit having been exceeded. These limits can be configured in the sensor setup in a way that adapts the Heartbeat diagnostics to the application.

#### Heartbeat and NAMUR category

The Heartbeat status indicates the sensor or device condition while the NAMUR categories (F, C, M, S) assess the reliability of the measured value. The two conditions can correlate but do not have to.

##### ■ Example 1

- The number of remaining cleaning cycles for the sensor reaches 20% of the defined maximum number. The Heartbeat symbol changes from ☺ to ☹. The measured value is still reliable so the NAMUR status signal does not change.
- If the maximum number of cleaning cycles is exceeded, the Heartbeat symbol changes from ☹ to ☹. While the measured value can still be reliable, the NAMUR status signal changes to M (maintenance required).

##### ■ Example 2

The sensor breaks. The Heartbeat status changes immediately from ☺ to ☹ and the NAMUR status signal also changes immediately to F (failure).

#### Heartbeat Monitoring

Sensor data from Memosens sensors are transmitted via the EtherNet/IP and Modbus TCP fieldbus protocols. These data can be used for predictive maintenance, for instance.

Examples include:

- Total hours of operation
- Hours of operation with very high or very low measured values
- Hours of operation at high temperatures
- Number of steam sterilizations
- Sensor identification
- Calibration information



SD EtherNet/IP and Modbus

#### Heartbeat Verification

Heartbeat Verification makes it possible to verify the correct operation of the measuring device without interrupting the process. This verification can be documented anytime.

#### Sensor Check System (SCS)

The Sensor Check System (SCS) monitors the high impedance of the pH glass. An alarm is issued if a minimum impedance value is undershot or a maximum impedance is exceeded.

- Glass breakage is the main reason for a drop in high impedance values
- The reasons for increasing impedance values include:
  - Dry sensor
  - Worn pH glass membrane



For the SCS, upper and lower limit values can be enabled or disabled independently of one another.

#### Process Check System (PCS)

The process check system (PCS) checks the measuring signal for stagnation. An alarm is triggered if the measuring signal does not change over a specific period (several measured values).

The main causes of stagnating measured values are:

- Contaminated sensor, or sensor outside of medium
- Sensor defective
- Process error (e.g. through control system)

#### Self-monitoring functions

Current inputs are deactivated in the event of overcurrent and reactivated once the overcurrent stops. Board voltages are monitored and the board temperature is also measured.

### USP and EP

The limit functions for pharmaceutical water in accordance with USP and EP specifications are implemented in the software for conductivity measurements:

- "Water for Injection" (WFI) as per USP <645> and EP
- "Highly Purified Water" (HPW) as per EP
- "Purified Water" (PW) as per EP

The uncompensated conductivity value and the temperature are measured for the USP/EP limit functions. The measured values are compared against the tables defined in the standards. An alarm is triggered if the limit value is exceeded. Furthermore, it is also possible to configure an early warning alarm that signals undesired operating states before they occur.

### ChemocleanPlus

Freely programmable sequence control


- e.g. for automatic sensor cleaning in retractable assemblies for reliable measurement results in processes with a high risk of contamination
- Individual, time-based activation of 4 outputs e.g. relays
- Starting, stopping or pausing of activities via digital input or fieldbus signals e.g. from limit position switches

## Maintainability


### Modular design

The modular transmitter design means it can be easily adapted to suit your needs:

- Retrofit extension modules for new or extended range of functions, e.g. current outputs, relays and digital communication
- Upgrade to maximum eight-channel measurement
- Optional: M12 sensor connector for connecting any kind of Memosens sensor
- Optional: CDI connector for external access to the service interface (avoids having to unscrew the housing cover)

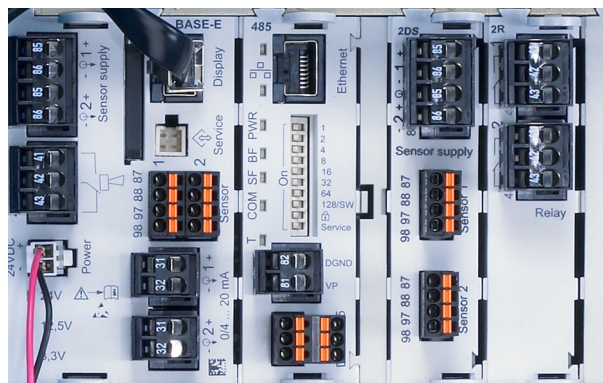

9 CM444R: example

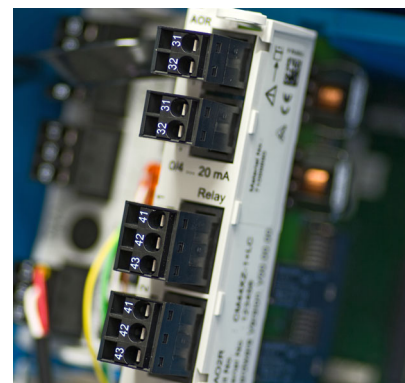


10 Extension module




### Data logger function

- Adjustable scan time: 1 to 3600 s (1 h)
- Data logbooks:
  - Max. 8 data logbooks
  - 150,000 entries per logbook
  - Graphic display (load curves) or numerical list
- Calibration logbook: max. 75 entries
- Hardware version logbook:
  - Hardware configuration and modifications
  - Max. 125 entries
- Version logbook:
  - E.g. software updates
  - Max. 50 entries
- Operation logbook: max. 250 entries
- Diagnostics logbook: max. 250 entries

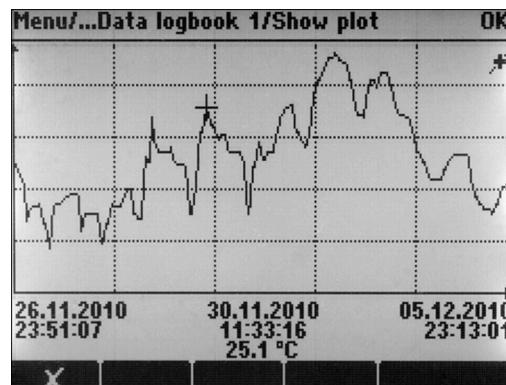

A0015032

11 Data logbook: Graphic display

 Logbooks remain unchanged even after a software update.

### SD card

The exchangeable storage medium enables:

- Quick and easy software updates and upgrades
- Data storage of internal device memory (e.g. logbooks)
- Transfer of complete configurations to a device with an identical setup (backup function)
- Transfer of configurations without the TAG and bus address to devices with an identical setup (copy function)
- Saving of screenshots for documentation purposes

Endress+Hauser offers industry-approved SD cards as accessories. These memory cards provide maximum data security and integrity.

Other SD cards up to a maximum weight of 5 g can also be used. However, Endress+Hauser does not accept any responsibility for the data security of such cards.

### External signals for device control and for activating external devices

Hardware options, e.g. module "DIO" with 2 digital inputs and 2 digital outputs or fieldbus module "485" enable the following:

- via a digital input signal
  - measuring range switching for conductivity (upgrade code required, see accessories)
  - switching between different calibration datasets in the case of optical sensors
  - an external hold
  - a cleaning interval to be triggered
  - switching on and off a PID controller, e.g. via the proximity switch of the CCA250
  - the use of the input as an "analog input" for pulse-frequency modulation (PFM)
- via a digital output signal
  - the static transmission (similar to a relay) of diagnostic states, point level switch states etc.
  - the dynamic transmission (comparable to a non-wearing "analog output") of PFM signals, e.g. to control dosing pumps.

## FieldCare and Field Data Manager

### FieldCare


Configuration and asset management software based on FDT/DTM technology

- Complete device configuration when connected via FXA291 and service interface
- Access to a number of configuration parameters and identification, measuring and diagnostic data when connected via HART modem
- Logbooks can be downloaded in CSV format or binary format for "Field Data Manager" software

### Field Data Manager

Visualization software and database for measuring, calibration and configuration data

- SQL database which is protected against manipulation
- Functions to import, save and print out logbooks
- Load curves to display measured values

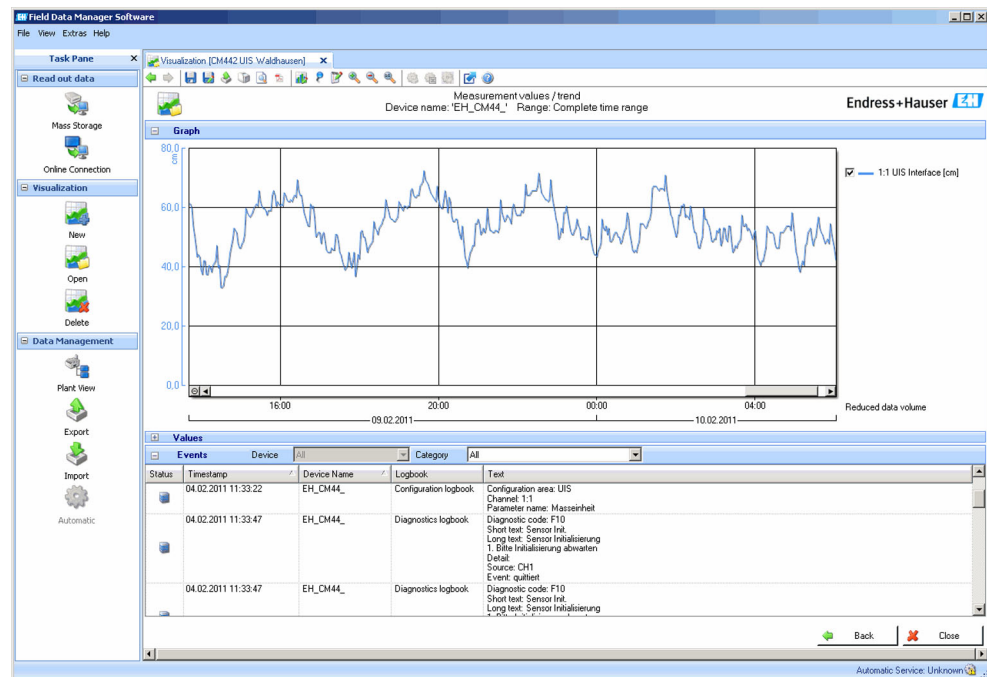

A0016009

12 Field Data Manager: Load curves

### Virtual process values (mathematical functions)

In addition to "real" process values, which are provided by connected physical sensors or analog inputs, mathematical functions can be used to calculate a maximum of 6 "virtual" process values.

The "virtual" process values can be:

- Output via a current output or a fieldbus
- Used as a controlled variable
- Assigned as a measured variable to a limit switch
- Used as a measured variable to trigger cleaning
- Displayed in user-defined measuring menus

The following mathematical functions are possible:

- Calculation of pH from two conductivity values according to VGB 405 RL, e. g. in boiler feedwater
- Difference between two measured values from different sources, e. g. for membrane monitoring
- Differential conductivity, e. g. for monitoring the efficiency of ion exchangers
- Degassed conductivity, e. g. for process controls in power plants
- Redundancy for monitoring two or three redundant sensors
- rH calculation based on the measured values of a pH and an ORP sensor
- Calculation of the remaining capacity of a cation exchanger
- Formula editor

**Concentration tables**

When the device is delivered from the factory, tables are saved in the device that allow inductive conductivity measurements to be converted to concentrations of certain substances. 4 user-defined tables are also possible.

*The following factory concentration tables are available:*

NaOH	0 to 15 %	0 to 100 °C (32 to 212 °F)
NaOH	25 to 50%	2 to 80 °C (36 to 176 °F)
HCl	0 to 20 %	0 to 65 °C (32 to 149 °F)
HNO <sub>3</sub>	0 to 30 %	2 to 80 °C (36 to 176 °F)
H <sub>2</sub> SO <sub>4</sub>	0.5 to 27 % and 35 to 85 %	0 to 100 °C (32 to 212 °F)
H <sub>2</sub> SO <sub>4</sub>	93 to 100 %	10 to 115 °C (50 to 239 °F)
H <sub>3</sub> PO <sub>4</sub>	0 to 40 %	2 to 80 °C (36 to 176 °F)
NaCl	0 to 26 %	2 to 80 °C (36 to 176 °F)

---

**Safety****Real-time clock**

The device has a real-time clock, which is buffered by a button cell battery if the power supply fails.

This ensures that the device continues to keep the correct date and time when it is restarted and that the time stamp for the logbooks is correct.

**Data security**

All settings, logbooks etc. are stored in a non-volatile memory to ensure that the data are retained even in the event of a disruption to the power supply.

**Measuring range switching for conductivity**

- Can be used in CIP processes e.g. for safe monitoring of phase separations
- Switching between 4 complete parameter sets:
  - Conductivity operating mode
  - Concentration tables
  - Temperature compensation
  - Output signal range
  - Limit value switch
- Via digital inputs or fieldbus

**Measured value compensation for oxygen and conductivity**

- Pressure or temperature compensation
- Input signals from external sensors via current input or fieldbus
- Signals from connected temperature sensors

**Password protection**

Password-protected login

- For remote operation via web server
- For local operation

**Process safety**

Two independent PID controllers

- One- or two-sided control
- Limit switches
- 4 cleaning programs which can be programmed independently of each other

**IT security**

Our warranty is valid only if the device is installed and used as described in the Operating Instructions. The device is equipped with security mechanisms to protect it against any inadvertent changes to the settings.

IT security measures, which provide additional protection for the device and associated data transfer, must be implemented by the operators themselves in line with their security standards.

## Input

<b>Measured variables</b>	→ Documentation of the connected sensor
<b>Measuring ranges</b>	→ Documentation of the connected sensor
<b>Types of input</b>	<ul style="list-style-type: none"> <li>▪ Digital sensor inputs for sensors with Memosens protocol</li> <li>▪ Analog current inputs (optional)</li> <li>▪ Digital inputs (optional)</li> </ul>
<b>Input signal</b>	Depending on version: <ul style="list-style-type: none"> <li>▪ Max. 8 x binary sensor signal</li> <li>▪ 2 x 0/4 to 20 mA (optional), passive, potentially isolated from one another and from the sensor inputs</li> <li>▪ 0 to 30 V</li> </ul>
<b>Cable specification</b>	<p><b>Cable type</b></p> Memosens data cable CYK10 or sensor fixed cable, each with cable end sleeves or M12 round-pin connector (optional)
	<p><b>Cable length</b></p> Max. 100 m (330 ft)

## Digital inputs, passive

<b>Electrical specification</b>	<ul style="list-style-type: none"> <li>▪ drawing power (passive)</li> <li>▪ Galvanically isolated</li> </ul>
<b>Span</b>	<ul style="list-style-type: none"> <li>▪ High: 11 to 30 V DC</li> <li>▪ Low: 0 to 5 V DC</li> </ul>
<b>Nominal input current</b>	max. 8 mA
<b>PFM function</b>	Minimum pulse width: 500 µs (1 kHz)
<b>Test voltage</b>	500 V
<b>Cable specification</b>	Max. 2.5 mm <sup>2</sup> (14 AWG)

## Current input, passive

<b>Span</b>	> 0 to 20 mA
<b>Signal characteristic</b>	Linear
<b>Internal resistance</b>	Non-linear
<b>Test voltage</b>	500 V

## Output

### Output signal

Depending on version:

- 2 x 0/4 to 20 mA, active, galvanically isolated from one another and from the sensor circuits
- 4 x 0/4 to 20 mA, active, galvanically isolated from one another and from the sensor circuits
- 6 x 0/4 to 20 mA, active, galvanically isolated from one another and from the sensor circuits
- 8 x 0/4 to 20 mA, active, galvanically isolated from one another and from the sensor circuits
- Optional HART communication (only via current output 1:1)

HART	
Signal encoding	FSK $\pm$ 0.5 mA above current signal
Data transmission rate	1200 baud
Galvanic isolation	Yes
Load (communication resistor)	250 $\Omega$

PROFIBUS DP/RS485	
Signal encoding	EIA/TIA-485, PROFIBUS DP-compliant acc. to IEC 61158
Data transmission rate	9.6 kBd, 19.2 kBd, 45.45kBd, 93.75 kBd, 187.5 kBd, 500 kBd, 1.5 MBd, 6 MBd, 12 MBd
Galvanic isolation	Yes
Connectors	Spring terminal (max. 1.5 mm), bridged internally (T-function), optional M12
Bus termination	Internal slide switch with LED display

Modbus RS485	
Signal encoding	EIA/TIA-485
Data transmission rate	2,400, 4,800, 9,600, 19,200, 38,400, 57,600 and 115,200 baud
Galvanic isolation	Yes
Connectors	Spring terminal (max. 1.5 mm), bridged internally (T-function), optional M12
Bus termination	Internal slide switch with LED display

Ethernet and Modbus TCP	
Signal encoding	IEEE 802.3 (Ethernet)
Data transmission rate	10/100 MBd
Galvanic isolation	Yes
Connection	RJ45
IP address	DHCP (default) or configuration via menu

EtherNet/IP	
Signal encoding	IEEE 802.3 (Ethernet)
Data transmission rate	10/100 MBd
Galvanic isolation	Yes
Connection	RJ45
IP address	DHCP (default) or configuration via menu

<b>Signal on alarm</b>	Adjustable, as per NAMUR Recommendation NE 43 <ul style="list-style-type: none"> <li>▪ In measuring range 0 to 20 mA (HART is not available with this measuring range): Failure current from 0 to 23 mA</li> <li>▪ In measuring range 4 to 20 mA: Failure current from 2.4 to 23 mA</li> <li>▪ Factory setting for failure current for both measuring ranges: 21.5 mA</li> </ul>
------------------------	--

<b>Load</b>	Max. 500 $\Omega$
-------------	-------------------

<b>Linearization/transmission behavior</b>	Linear
--	--------

## Digital outputs, passive

<b>Electrical specification</b>	<ul style="list-style-type: none"> <li>▪ Passive</li> <li>▪ Open collector, max. 30 V, 15 mA</li> <li>▪ Maximum voltage drop 3 V</li> </ul>
---------------------------------	---

<b>External power supply</b>	When using an onsite auxiliary voltage supply and an onsite digital input: Recommended minimum auxiliary voltage = 3 V + $V_{IHmin}$ ( $V_{IHmin}$ = minimum input voltage required (high-level input voltage))
------------------------------	---

<b>PFM function</b>	Minimum pulse width: 500 $\mu$ s (1 kHz)
---------------------	--

<b>Auxiliary voltage</b>	<b>Electrical specification</b> <ul style="list-style-type: none"> <li>▪ Galvanically isolated</li> <li>▪ Unregulated, 24 V DC</li> <li>▪ Max. 50 mA (per DIO module)</li> </ul>
--------------------------	--

<b>Test voltage</b>	500 V
---------------------	-------

<b>Cable specification</b>	Max. 2.5 mm <sup>2</sup> (14 AWG)
----------------------------	-----------------------------------

## Current outputs, active

<b>Span</b>	0 to 23 mA 2.4 to 23 mA for HART communication
-------------	---

<b>Signal characteristic</b>	Linear
------------------------------	--------

<b>Electrical specification</b>	<b>Output voltage</b> Max. 24 V  <b>Test voltage</b> 500 V
---------------------------------	--

<b>Cable specification</b>	<b>Cable type</b> Recommended: shielded cable  <b>Cable specification</b> Max. 2.5 mm <sup>2</sup> (14 AWG)
----------------------------	---

## Relay outputs

### Electrical specification

#### Relay types

- 1 single-pin changeover contact (alarm relay)
- 2 or 4 single-pin changeover contacts (optional with extension modules)

#### Maximum load

- Alarm relay: 0.5 A
- All other relays: 2.0 A

#### Relay switching capacity

##### Base module (Alarm relay)

Switching voltage	Load (max.)	Switching cycles (min.)
230 V AC, $\cos\Phi = 0.8$ to 1	0.1 A	700,000
	0.5 A	450,000
115 V AC, $\cos\Phi = 0.8$ to 1	0.1 A	1,000,000
	0.5 A	650,000
24 V DC, L/R = 0 to 1 ms	0.1 A	500,000
	0.5 A	350,000

##### Extension modules

Switching voltage	Load (max.)	Switching cycles (min.)
230 V AC, $\cos\Phi = 0.8$ to 1	0.1 A	700,000
	0.5 A	450,000
	2 A	120,000
115 V AC, $\cos\Phi = 0.8$ to 1	0.1 A	1,000,000
	0.5 A	650,000
	2 A	170,000
24 V DC, L/R = 0 to 1 ms	0.1 A	500,000
	0.5 A	350,000
	2 A	150,000

### Cable specification

Max. 2.5 mm<sup>2</sup> (14 AWG)

## Protocol-specific data

### HART

Manufacturer ID	11 <sub>h</sub>
Device type	155D <sub>h</sub>
Device revision	001 <sub>h</sub>
HART version	7.2
Device description files (DD/DTM)	<a href="http://www.endress.com/hart">www.endress.com/hart</a> Device Integration Manager DIM
Device variables	16 user-definable and 16 predefined device variables, dynamic variables PV, SV, TV, QV
Supported features	PDM DD, AMS DD, DTM, Field Xpert DD

**PROFIBUS DP**

Manufacturer ID	11 <sub>h</sub>
Device type	155D <sub>h</sub>
Profile version	3.02
GSD files	<a href="http://www.endress.com/profibus">www.endress.com/profibus</a> Device Integration Manager DIM
Output values	16 AI blocks, 8 DI blocks
Input variables	4 AO blocks, 8 DO blocks
Supported features	<ul style="list-style-type: none"> <li>▪ 1 MSCY0 connection (cyclical communication, master class 1 to slave)</li> <li>▪ 1 MSAC1 connection (acyclical communication, master class 1 to slave)</li> <li>▪ 2 MSAC2 connections (acyclical communication, master class 2 to slave)</li> <li>▪ Device lock: The device can be locked using the hardware or software.</li> <li>▪ Addressing using DIL switches or software</li> <li>▪ GSD, PDM DD, DTM</li> </ul>

**Modbus RS485**

Protocol	RTU/ASCII
Function codes	03, 04, 06, 08, 16, 23
Broadcast support for function codes	06, 16, 23
Output data	16 measured values (value, unit, status), 8 digital values (value, status)
Input data	4 setpoints (value, unit, status), 8 digital values (value, status), diagnostic information
Supported features	Address can be configured using switch or software

**Modbus TCP**

TCP port	502
TCP connections	3
Protocol	TCP
Function codes	03, 04, 06, 08, 16, 23
Broadcast support for function codes	06, 16, 23
Output data	16 measured values (value, unit, status), 8 digital values (value, status)
Input data	4 setpoints (value, unit, status), 8 digital values (value, status), diagnostic information
Supported features	Address can be configured using DHCP or software

**EtherNet/IP**

Log	EtherNet/IP	
ODVA certification	Yes	
Device profile	Generic device (product type: 0x2B)	
Manufacturer ID	0x049E <sub>h</sub>	
Device type ID	0x109C <sub>h</sub>	
Polarity	Auto-MIDI-X	
Connections	CIP	12
	I/O	6
	Explicit message	6
	Multicast	3 consumers
Minimum RPI	100 ms (default)	



Maximum RPI	10000 ms	
System integration	EtherNet/IP	EDS
	Rockwell	Add-on-Profile Level 3, Faceplate for Factory Talk SE
IO data	Input (T → O)	Device status and diagnostic message with highest priority Measured values: <ul style="list-style-type: none"> <li>▪ 16 AI (analog input) + Status + Unit</li> <li>▪ 8 DI (discrete input) + Status</li> </ul>
	Output (O → T)	Actuating values: <ul style="list-style-type: none"> <li>▪ 4 AO (analog output) + status + unit</li> <li>▪ 8 DO (discrete output) + Status</li> </ul>

**Web server**

The Web server enables full access to the device configuration, measured values, diagnostic messages, logbooks and service data via standard WiFi/WLAN/LAN/GSM or 3G routers with a user-defined IP address.

TCP port	80
Supported features	<ul style="list-style-type: none"> <li>▪ Remote-controlled device configuration(1 session)</li> <li>▪ Save/restore device configuration (via SD card)</li> <li>▪ Logbook export (file formats: CSV, FDM)</li> <li>▪ Access to Web server via DTM or Internet Explorer</li> <li>▪ Login</li> <li>▪ Web server can be switched off</li> </ul>

## Power supply

**Supply voltage**

**CM442 R**

Depending on version:

- 100 to 230 V AC, 50/60 Hz  
Maximum permitted fluctuation of mains supply voltage: ± 15 % of nominal voltage
- 24 V AC/DC, 50/60 Hz  
Maximum permitted fluctuation of mains supply voltage: + 20/- 15 % of nominal voltage

**CM444 R and CM448 R**

Depending on the version, via external DIN rail power unit:

- 100 to 230 V AC, 50/60 Hz  
Maximum permitted fluctuation of mains supply voltage: ± 15 % of nominal voltage <sup>1)</sup>
- 24 V DC  
Maximum permitted fluctuation of mains supply voltage: + 20/- 15 % of nominal voltage <sup>1)</sup>

**NOTICE**

**The device does not have a power switch!**

- ▶ Provide a protected circuit breaker in the vicinity of the device at the place of installation.
- ▶ The circuit breaker must be a switch or power switch, and must be labeled as the circuit breaker for the device.
- ▶ At the supply point, the power supply must be isolated from dangerous live cables by double or reinforced insulation in the case of devices with a 24 V supply voltage.

**Power consumption**

**CM442 R**

Depending on supply voltage

- 100 to 230 V AC and 24 V AC:  
Max. 55 VA
- 24 V DC:  
Max. 22 W

1) \*Specifications only apply if used with power unit supplied by manufacturer.

**CM444 R and CM448 R**

Depending on supply voltage

- 100 to 230 V AC:  
Max. 150 VA
- 24 V DC:  
Max. 59 W

**Fuse** Fuse not exchangeable


**Overvoltage protection** Integrated overvoltage/lightning protection as per EN 61326  
Protection category 1 and 3

**Cable specification for optional display cable**


**Length of display cable provided:**  
3 m (10 ft)

**Maximum permitted length of a display cable:**  
5 m (16.5 ft)

**Electrical connection** **Basic module**

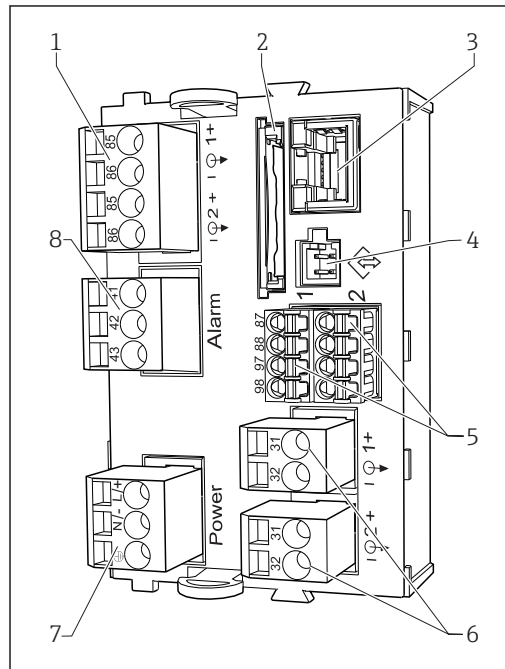

A0012405

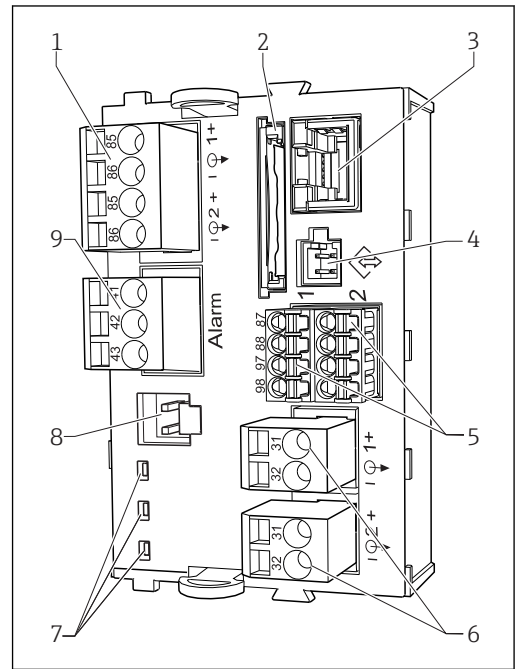

A0015871

■ 13 Basic module BASE-H or -L (two-channel device)

- 1 Power supply for digital fixed cable sensors with Memosens protocol
- 2 SD card slot
- 3 Slot for display cable <sup>1)</sup>
- 4 Service interface
- 5 Connections for 2 Memosens sensors
- 6 Current outputs
- 7 LEDs
- 8 Alarm relay connection


■ 14 Basic module BASE-E (four- and eight-channel device)

- 1 Power supply for digital fixed cable sensors with Memosens protocol
- 2 SD card slot
- 3 Slot for display cable <sup>1)</sup>
- 4 Service interface
- 5 Connections for 2 Memosens sensors
- 6 Current outputs
- 7 LEDs
- 8 Socket for internal supply cable <sup>2)</sup>
- 9 Alarm relay connection


<sup>1)</sup> For optional external display.

<sup>2)</sup> Power supply to DIN rail power unit.

Connecting supply voltage for CM442R

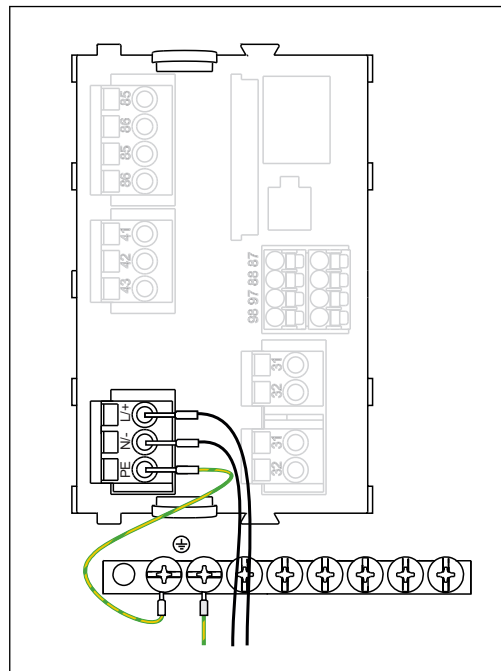

A0025364

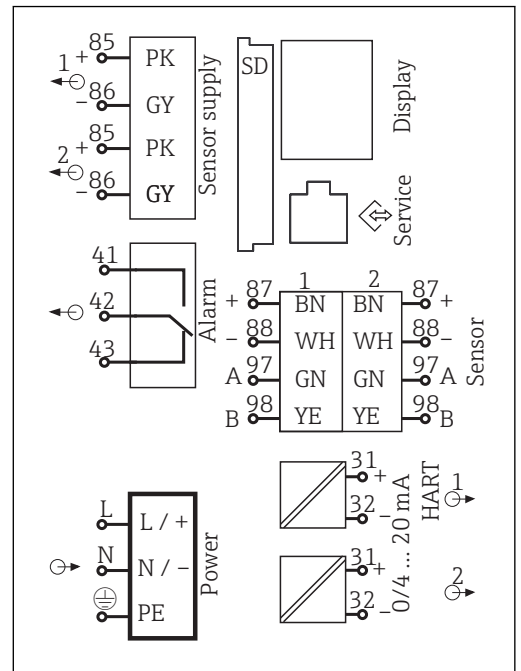


A0012404

15 Connecting power supply on the BASE-H or -L


16 Overall wiring diagram for BASE-H or -L

H Power unit 100 to 230 VAC  
L Power unit 24 VAC or 24 VDC

Connecting supply voltage for CM444R and CM448R

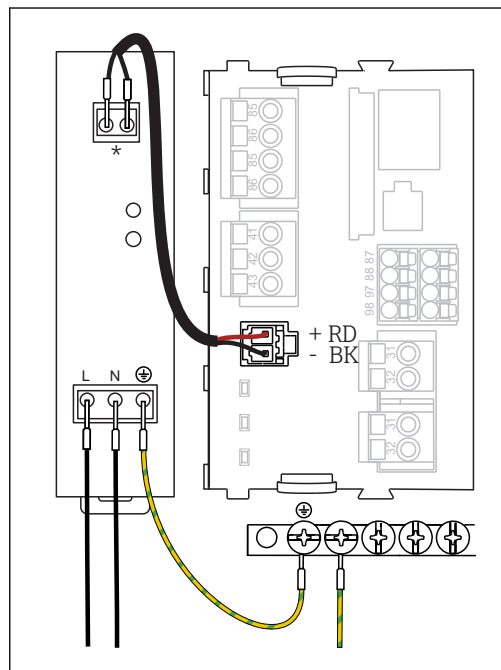

A0025365

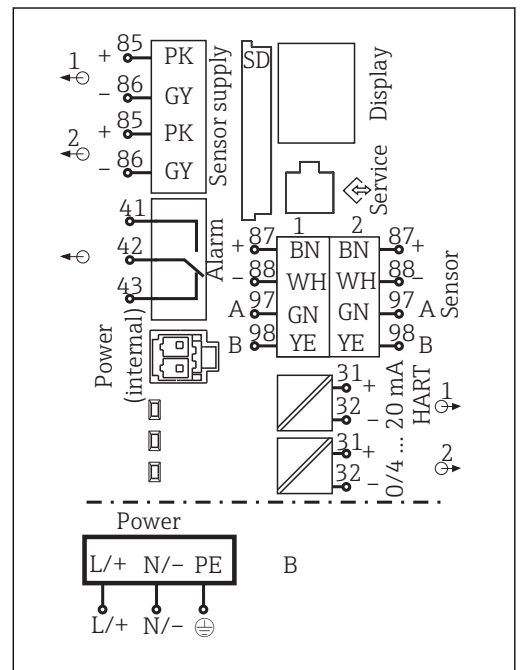

A0015873

17 Connecting power supply with BASE-E

18 Overall wiring diagram BASE-E and external power unit (B)

\* Assignment depending on power unit, make sure to connect correctly

**i** The two device versions may only be operated with the power unit supplied and the power unit cable. Also pay attention to the information in the operating manual supplied for the power unit.

Connecting optional modules

With extension modules you can purchase additional functions for your device.

**NOTICE**

**Unacceptable hardware combinations (due to conflicts in power supply)**

Incorrect measurements or total failure of the measuring point as a result of heat build-up or overloading

- ▶ If you are planning to extend your controller, make sure the resulting hardware combination is permitted (Configurator at [www.endress.com/CM442R](http://www.endress.com/CM442R) or .../CM444R or .../CM448R).
- ▶ Remember that the sum of all current inputs and outputs may not exceed 8.
- ▶ Make sure not to use more than 2 "DIO" modules. More "DIO" modules are not permitted.
- ▶ Please contact your Endress+Hauser sales center should you have any questions.

Overview of all the modules available


Module name				
AOR	2R	4R	2DS	DIO
<ul style="list-style-type: none"> <li>■ 2 x 0/4 to 20 mA analog outputs</li> <li>■ 2 relays</li> <li>■ Order No. 71111053</li> </ul>	<ul style="list-style-type: none"> <li>■ 2 relays</li> <li>■ Order No. 71125375</li> </ul>	<ul style="list-style-type: none"> <li>■ 4 relays</li> <li>■ Order No. 71125376</li> </ul>	<ul style="list-style-type: none"> <li>■ 2 digital sensor inputs</li> <li>■ 2 power supply systems for digital sensors</li> <li>■ Order No. 71135631</li> </ul>	<ul style="list-style-type: none"> <li>■ 2 digital inputs</li> <li>■ 2 digital outputs with auxiliary voltage</li> <li>■ Order No. 71135638</li> </ul>

Module name				
2AO	4AO	2AI	485	ETH
<ul style="list-style-type: none"> <li>2 x 0/4 to 20 mA analog outputs</li> <li>Order No. 71135632</li> </ul>	<ul style="list-style-type: none"> <li>4 x 0/4 to 20 mA analog outputs</li> <li>Order No. 71135633</li> </ul>	<ul style="list-style-type: none"> <li>2 x 0/4 to 20mA analog inputs</li> <li>Order No. 71135639</li> </ul>	<ul style="list-style-type: none"> <li>Ethernet (web server or Modbus TCP)</li> <li>5V power supply for PROFIBUS DP termination</li> <li>RS485 (PROFIBUS DP or Modbus RS485)</li> <li>Order No. 71135634</li> </ul>	<ul style="list-style-type: none"> <li>Web server and Ethernet/IP or Modbus TCP</li> <li>Order No. 71272410</li> </ul>

**PROFIBUS DP (module 485)**

Contacts 95, 96 and 99 are bridged in the connector. This ensures that PROFIBUS communication is not interrupted if the connector is disconnected.

**Protective ground connection**

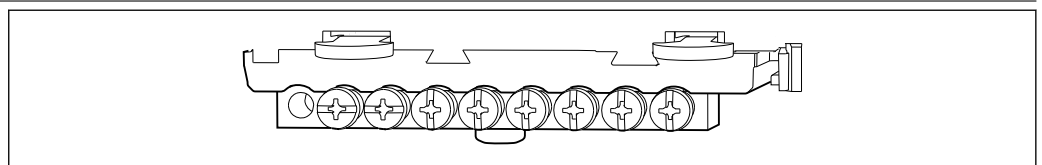

19 Mounting rail for functional ground connections

A0025366

**Sensor connection***Sensors with Memosens protocol*


Sensor types	Sensor cable	Sensors
Digital sensors <b>without</b> additional internal power supply	With plug-in connection and inductive signal transmission	<ul style="list-style-type: none"> <li>▪ pH sensors</li> <li>▪ ORP sensors</li> <li>▪ Combined sensors</li> <li>▪ Oxygen sensors (amperometric and optical)</li> <li>▪ Conductivity sensors with conductive measurement of conductivity</li> <li>▪ Chlorine sensors (disinfection)</li> </ul>
	Fixed cable	Conductivity sensors with inductive measurement of conductivity
Digital sensors with additional internal power supply	Fixed cable	<ul style="list-style-type: none"> <li>▪ Turbidity sensors</li> <li>▪ Sensors for interface measurement</li> <li>▪ Sensors for measuring the spectral absorption coefficient (SAC)</li> <li>▪ Nitrate sensors</li> <li>▪ Optical oxygen sensors</li> <li>▪ Ion-sensitive sensors</li> </ul>

**The following rule applies if connecting CUS71D sensors:**

- CM442R
  - Only one CUS71D is possible; an additional sensor is not permitted.
  - The second sensor input may also not be used for another type of sensor.
- CM444R
  - No restrictions. All the sensor inputs can be used as required.
- CM448R
  - If a CUS71D is connected, the number of sensor inputs that can be used is limited to a maximum of 4.
  - Of these, all 4 inputs can be used for CUS71D sensors.
  - Every combination of CUS71D and other sensors is possible, provided that the total number of connected sensors does not exceed 4.


**Connection**

Direct connection of sensor cable to terminal connector of the sensor module 2DS or of base module L, H or E (→  20 ff.)

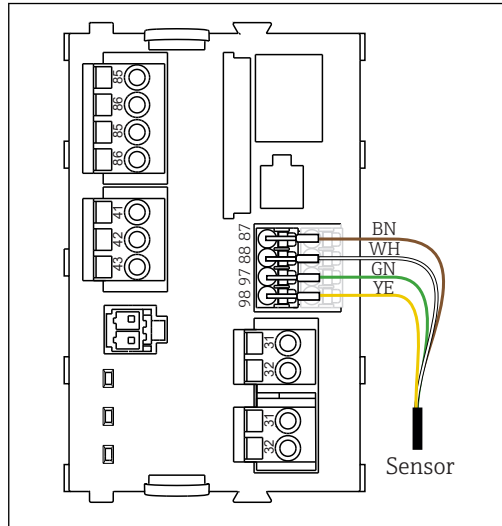


A0023038

20 sensors without additional supply voltage

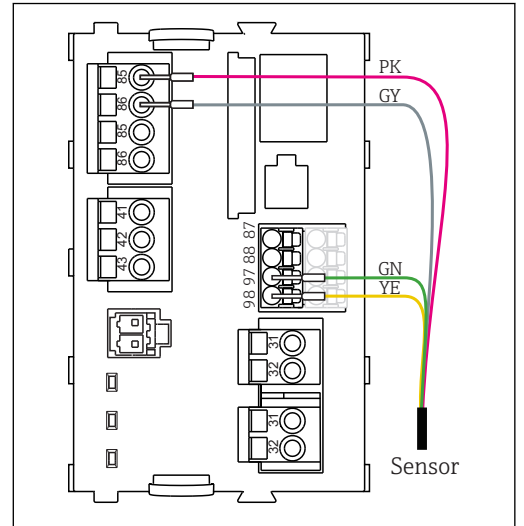

A0023039

21 sensors with additional supply voltage

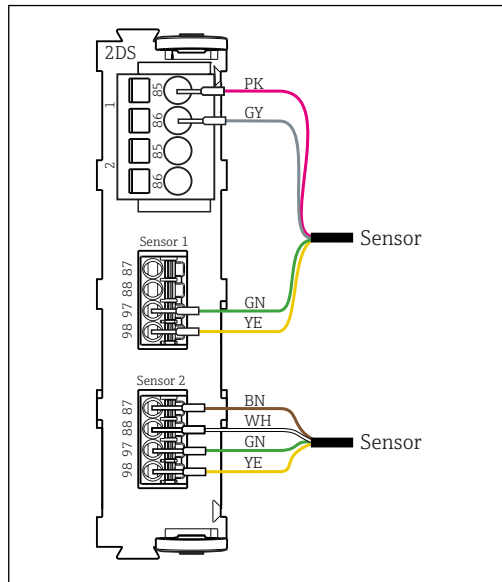

A0033206

22 sensors with and without additional supply voltage at sensor module 2DS

## Performance characteristics

<b>Response time</b>	<b>Current outputs</b> $t_{90}$ = max. 500 ms for an increase from 0 to 20 mA <b>Current inputs</b> $t_{90}$ = max. 330 ms for an increase from 0 to 20 mA <b>Digital inputs and outputs</b> $t_{90}$ = max. 330 ms for an increase from low to high
<b>Reference temperature</b>	25 °C (77 °F)
<b>Measured error for sensor inputs</b>	→ Documentation of the connected sensor
<b>Measured error for current inputs and outputs</b>	<b>Typical measured errors:</b> < 20 $\mu$ A (with current values < 4 mA) < 50 $\mu$ A (with current values 4 to 20 mA) at 25 °C (77 °F) each <b>Additional measured error depending on the temperature:</b> < 1.5 $\mu$ A/K
<b>Frequency tolerance of digital inputs and outputs</b>	$\leq 1\%$
<b>Resolution of current inputs and outputs</b>	< 5 $\mu$ A
<b>Repeatability</b>	→ Documentation of the connected sensor

## Installation

Mounting on DIN rail as per IEC 60715

### NOTICE

#### Incorrect mounting location in the cabinet, spacing regulations not observed


Possible malfunctions as a result of heat buildup and interference from neighboring devices!

- ▶ Do not position the device directly above sources of heat. The temperature specification must be observed.
- ▶ The components are designed for convection-based cooling. Avoid heat buildup. Ensure openings are not covered, e. g. by cables.
- ▶ Observe the specified distances to other devices.
- ▶ Physically separate the device from frequency converters and high-voltage devices.
- ▶ Recommended installation direction: horizontal. The specified ambient conditions, and particularly the ambient temperatures, only apply for horizontal installation.
- ▶ Vertical orientation is also possible. However, this requires additional fixing clips at the place of installation to hold the device in position on the DIN rail.
- ▶ Recommended installation of power unit for CM444R and CM448R: to the left of the device.



**The following minimum clearance specifications must be observed:**


- Distances at the side in relation to other devices incl. power units and to the wall of the cabinet:  
at least 20 mm (0.79 inch)
- Distance above and below the device and depth distance (to control cabinet door or other devices installed there):  
at least 50 mm (1.97 inch)

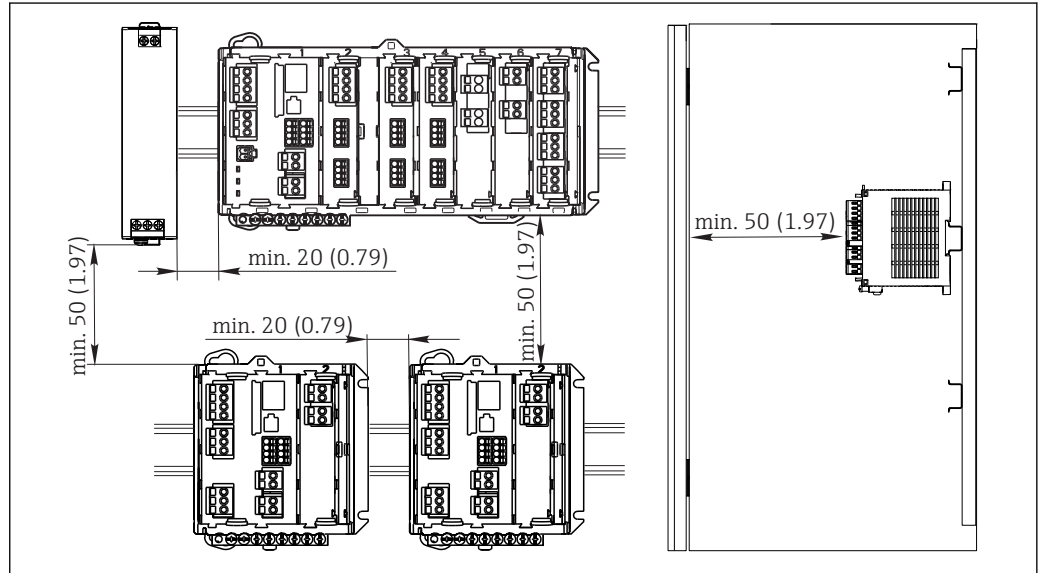

A0025369

23 Minimum clearance in mm (in)


**Wall mounting**

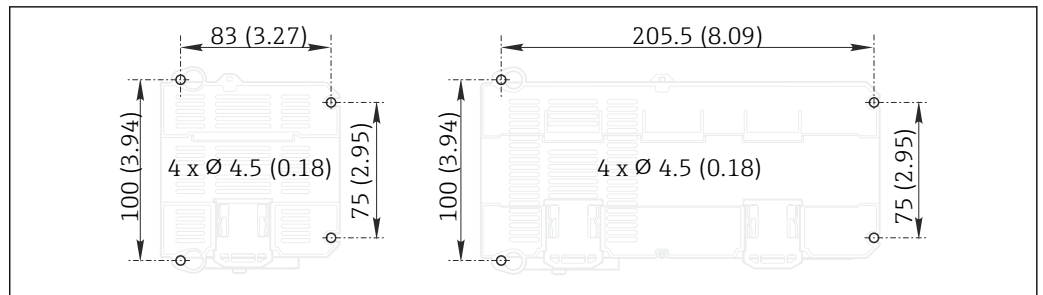


A0025370


24 Drilling pattern for wall mounting in mm (in)

**Mounting the external display**

 The mounting plate also serves as the drilling template. The marks on the side help you mark the position of the drill holes.

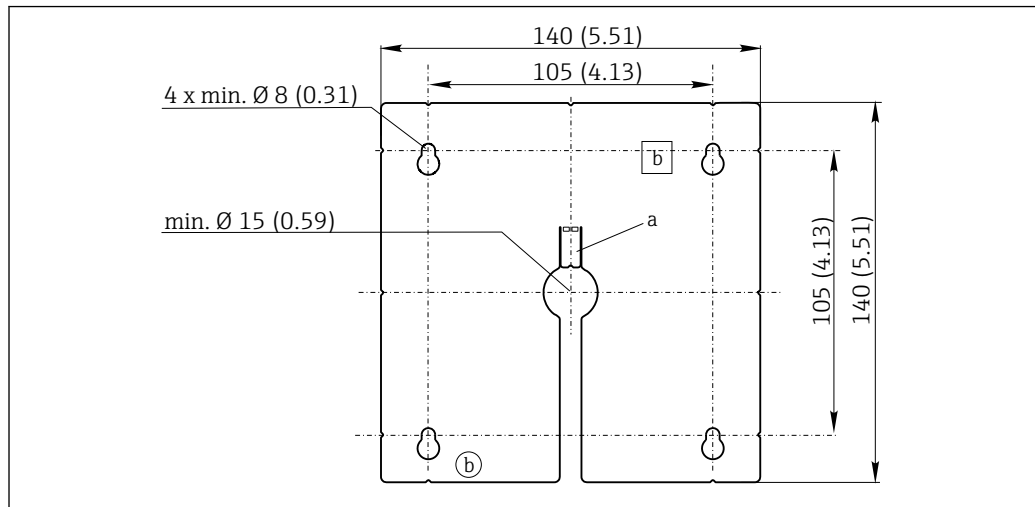

A0025371

 25 Mounting plate of external display, dimensions in mm (in)

a Retaining tab

b Production-related recesses, no function for the user

## Environment

### Ambient temperature range

#### CM442R

0 to 60 °C (32 to 140 °F)

#### CM444R

■ Generally 0 to 55 °C (32 to 130 °F), with the exception of packages under the second list item

■ 0 to 50 °C (32 to 120 °F) for the following packages:

- CM444R-\*\*M40A7FI\*+...
- CM444R-\*\*M40A7FK\*+...
- CM444R-\*\*M4AA5F4\*+...
- CM444R-\*\*M4AA5FF\*+...
- CM444R-\*\*M4AA5FH\*+...
- CM444R-\*\*M4AA5FI\*+...
- CM444R-\*\*M4AA5FK\*+...
- CM444R-\*\*M4AA5FM\*+...
- CM444R-\*\*M4BA5F4\*+...
- CM444R-\*\*M4BA5FF\*+...
- CM444R-\*\*M4BA5FH\*+...
- CM444R-\*\*M4BA5FI\*+...
- CM444R-\*\*M4BA5FK\*+...
- CM444R-\*\*M4BA5FM\*+...
- CM444R-\*\*M4DA5F4\*+...
- CM444R-\*\*M4DA5FF\*+...
- CM444R-\*\*M4DA5FH\*+...
- CM444R-\*\*M4DA5FI\*+...
- CM444R-\*\*M4DA5FK\*+...
- CM444R-\*\*M4DA5FM\*+...

**CM448R**

- Generally 0 to 55 °C (32 to 130 °F), with the exception of packages under the second list item
- 0 to 50 °C (32 to 120 °F) for the following packages:
  - CM448R-\*\*\*6AA\*+...
  - CM448R-\*\*\*8A4\*+...
  - CM448R-\*\*\*8A5\*+...
  - CM448R-\*\*28A3\*+...
  - CM448R-\*\*38A3\*+...
  - CM448R-\*\*48A3\*+...
  - CM448R-\*\*58A3\*+...
  - CM448R-\*\*68A3\*+...
  - CM448R-\*\*26A5\*+...
  - CM448R-\*\*36A5\*+...
  - CM448R-\*\*46A5\*+...
  - CM448R-\*\*56A5\*+...
  - CM448R-\*\*66A5\*+...
  - CM448R-\*\*22A7\*+...
  - CM448R-\*\*32A7\*+...
  - CM448R-\*\*42A7\*+...
  - CM448R-\*\*52A7\*+...
  - CM448R-\*\*62A7\*+...
  - CM448R-\*\*A6A5\*+...
  - CM448R-\*\*A6A7\*+...
  - CM448R-\*\*B6A5\*+...
  - CM448R-\*\*B6A7\*+...
  - CM448R-\*\*C6A5\*+...
  - CM448R-\*\*C6A7\*+...
  - CM448R-\*\*D6A5\*+...
  - CM448R-\*\*D6A7\*+...

**External display (optional)**

-20 to 60 °C (0 to 140 °F)

<b>Storage temperature</b>	-25 to 85 °C (-13 to 185 °F)													
<b>Humidity</b>	<b>DIN rail device</b> 5 to 85%, not condensing  <b>External display (in installed state)</b> 5 to 95%, not condensing													
<b>Degree of protection</b>	<b>DIN rail device</b> IP20 shock protection  <b>External display</b> IP66 front-panel, when installed correctly including seal for housing door													
<b>Climate class</b>	As per IEC 60654-1: B2													
<b>Vibration resistance</b>	<b>Environmental tests</b> Vibration test based on DIN EN 60068-2, October 2008 Vibration test based on DIN EN 60654-3, August 1998  <b>Wall mounting</b> <table border="0"> <tr> <td>Frequency range</td> <td colspan="2">10 to 150 Hz (sinusoidal)</td> </tr> <tr> <td>Amplitude</td> <td>10 to 12.9 Hz:</td> <td>0.75 mm</td> </tr> <tr> <td></td> <td>12.9 to 150 Hz:</td> <td>0.5 g<sup>1)</sup></td> </tr> <tr> <td>Test duration</td> <td colspan="2">10 frequency cycles/ spatial axis, in 3 spatial axes (1 oct./min)</td> </tr> </table> <p>1) g ... gravitational acceleration (1 g ≈ 9.81 m/s<sup>2</sup>)</p>		Frequency range	10 to 150 Hz (sinusoidal)		Amplitude	10 to 12.9 Hz:	0.75 mm		12.9 to 150 Hz:	0.5 g <sup>1)</sup>	Test duration	10 frequency cycles/ spatial axis, in 3 spatial axes (1 oct./min)	
Frequency range	10 to 150 Hz (sinusoidal)													
Amplitude	10 to 12.9 Hz:	0.75 mm												
	12.9 to 150 Hz:	0.5 g <sup>1)</sup>												
Test duration	10 frequency cycles/ spatial axis, in 3 spatial axes (1 oct./min)													
<b>Electromagnetic compatibility</b>	Interference emission and interference immunity as per EN 61326-1:2013, Class A for Industry													


**Electrical safety** IEC 61010-1, Class I equipment  
 Low voltage: overvoltage category II  
 Environment < 2000 m (< 6562 ft) above MSL

**Degree of contamination** DIN rail device  
 The product is suitable for pollution degree 2.

**Optional display**  
 The product is suitable for pollution degree 4.

## Mechanical construction


**Dimensions** CM442R

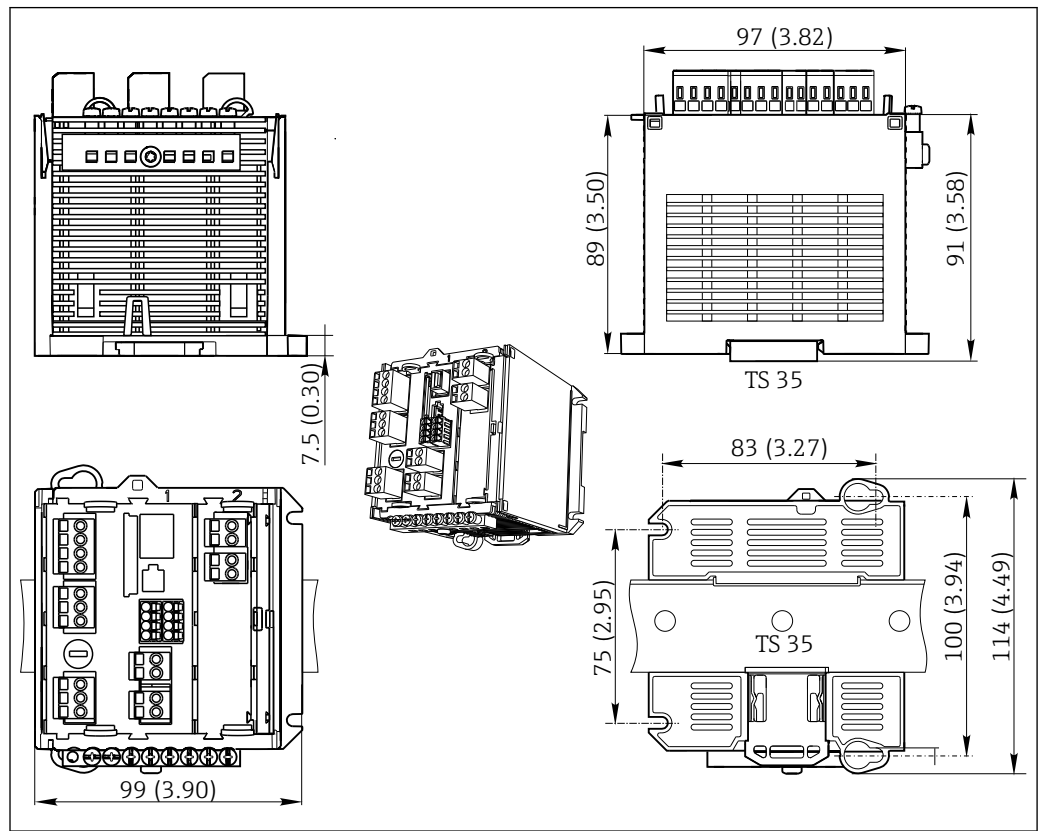

A0025344

26 Dimensions in mm (inch)


CM444R and CM448R

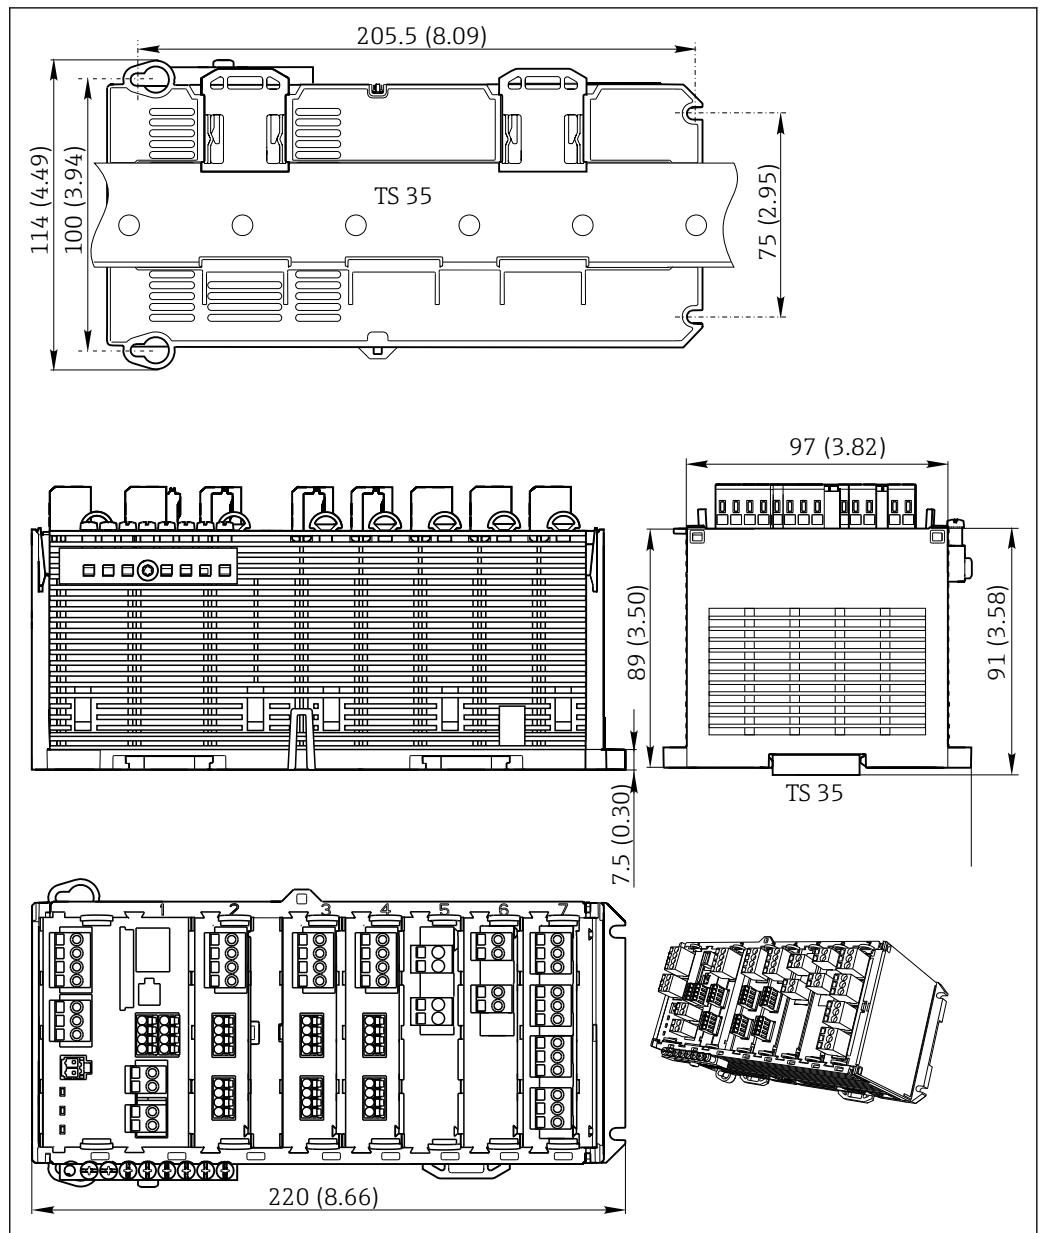

A0025345

27 Dimensions in mm (inch)

**Optional display**

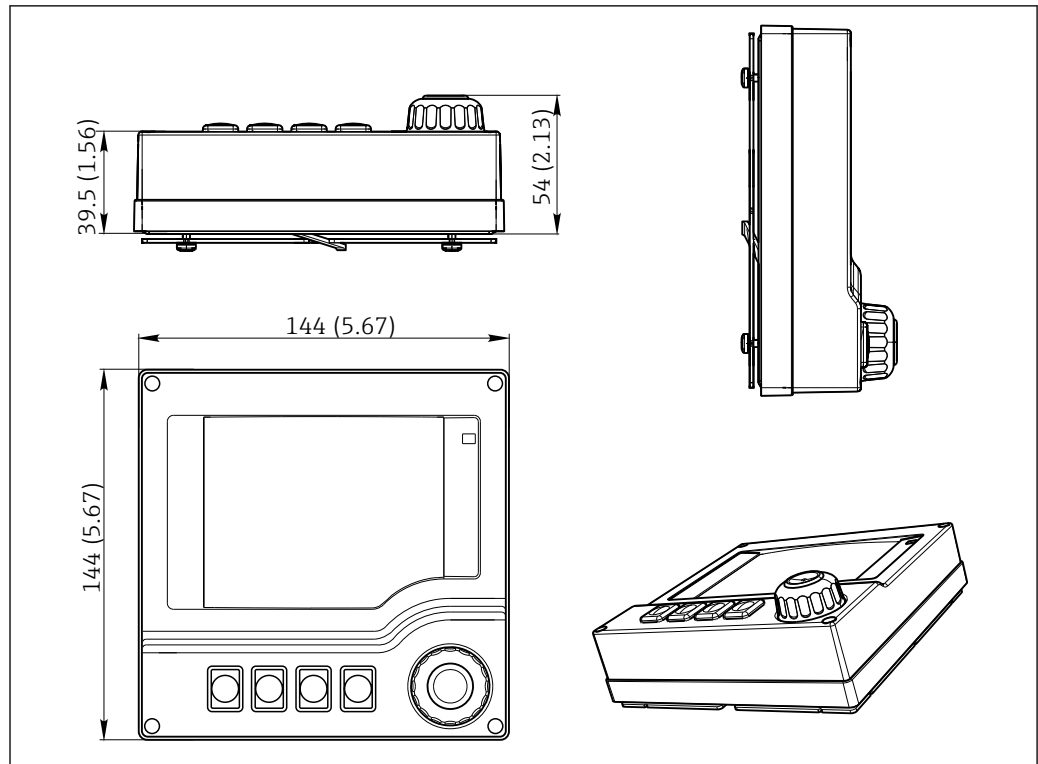


A0025346

28 Dimensions in mm (inch)


**External power units (CM444R and CM448R only)**

Depending on the version ordered, a power unit for connection to 230 V or 24 V is supplied. There are two delivery variants for each version (cannot be selected). The factory-preferred variant is shown on the left in each case.

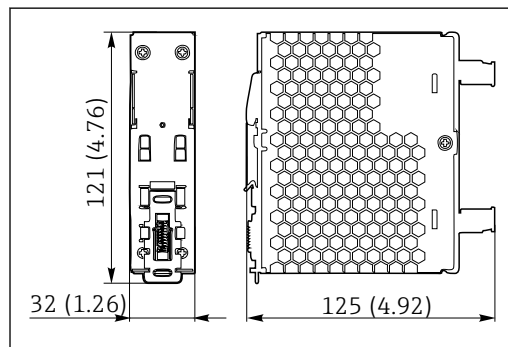


A0025738

29 Power unit 230 V

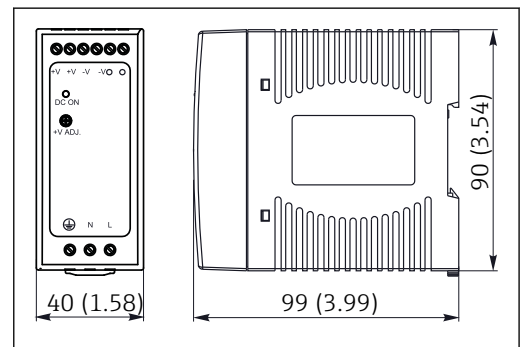


A0025739

30 Power unit 230 V (optional)

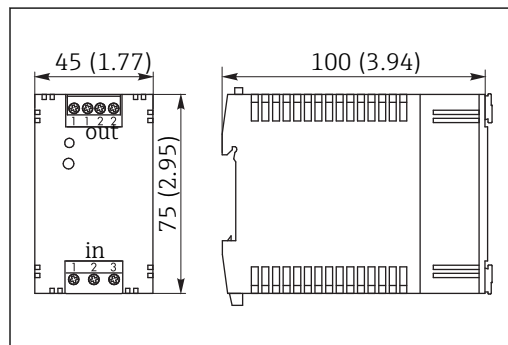

A0025784

31 Power unit 24 V

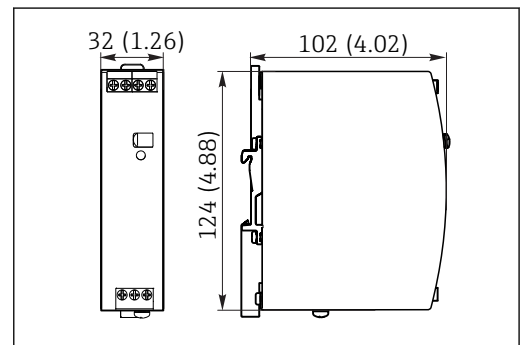


A0025786

32 Power unit 24 V (optional)

**Service display (accessories)**

The service display comprises:

- Portable display (same dimensions as under "Optional display")
- Cover to protect the display and to hook it onto the (open) cabinet door

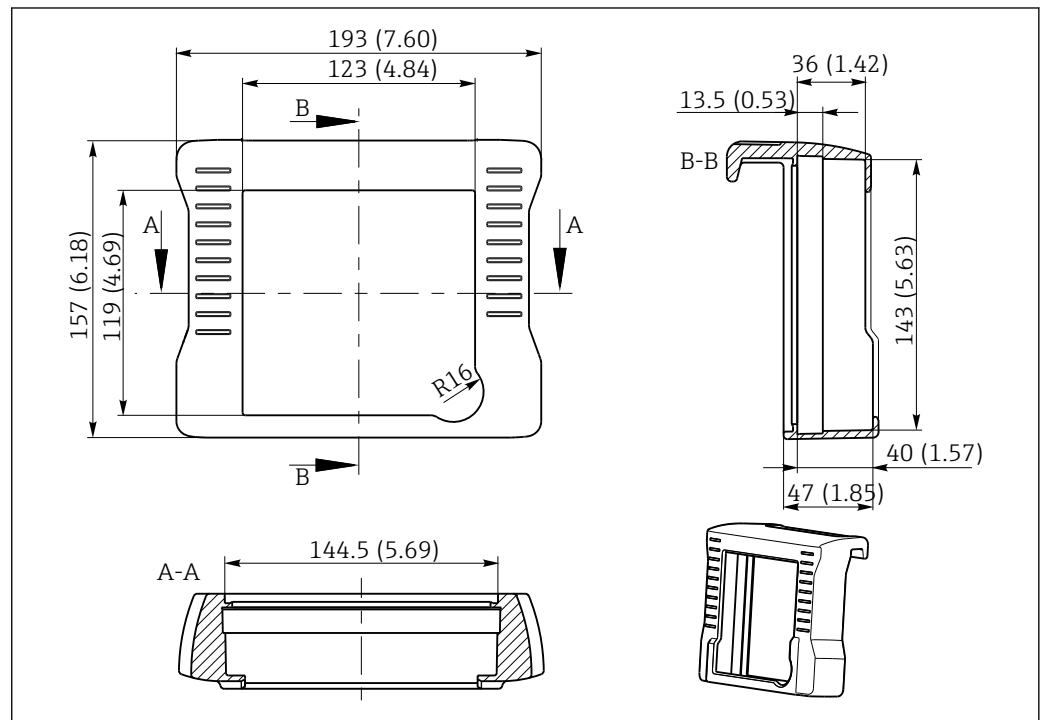

33 Dimensions of the service display cover in mm (inch)

A0025343

**Weight**

**depending on the version:**

CM442R (fully configured)	Approx. 0.45 kg (1 lbs)
CM444R and CM448R (fully configured)	Approx. 0.95 kg (2.1 lbs)
Individual module	Approx. 0.06 kg (0.13 lbs)
External display (excluding cables)	Approx. 0.56 kg (1.2 lbs)
Service display cover	0.46 kg (1 lbs)
External power unit (CM444R, CM448R)	0.27 to 0.42 kg (0.60 to 0.92 lbs), depending on the power unit variant
SD card	Max. 5 g (0.17 oz)

**Materials**

DIN rail housing	PC-FR
Display cover	PC-FR
Display seal	EPDM
Soft keys	EPDM
Module covers	PBT GF30 FR
Terminal strip	Nickel-plated brass
Ground terminals	Stainless steel 1.4301 (AISI304)
Threaded fasteners	Stainless steel 1.4301 (AISI304)
Mounting plate (optional display)	Stainless steel 1.4301 (AISI304)
Securing screws (optional display)	Steel, galvanized
Cover for service display (accessories)	EPDM

## Operability

### External display

Graphic display:

- Resolution: 240 x 160 pixel
- Back light with switch-off function
- Red display background for alarms alerts users to errors
- Transflective display technology for maximum contrast even in bright environments
- User-definable measuring menus mean you can always keep track of the values that are important for your application.

### Operating concept


The simple and structured operating concept sets new standards:

- Intuitive operation with the navigator and soft keys
- Fast configuration of application-specific measurement options
- Easy configuration and diagnosis thanks to plain-text display
- All languages that can be ordered are available in every device




A0025229

34 Operation via external, optional display

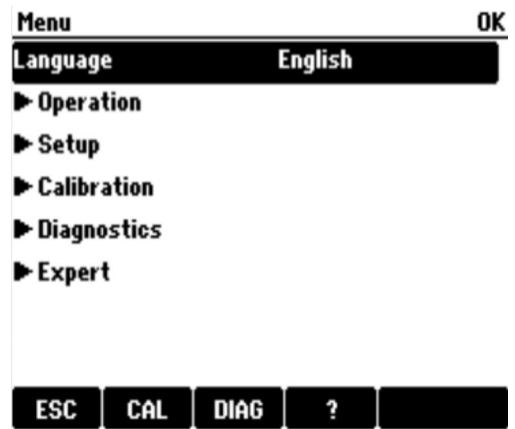

35 Plain-text menu

### Local operation via external, optional display

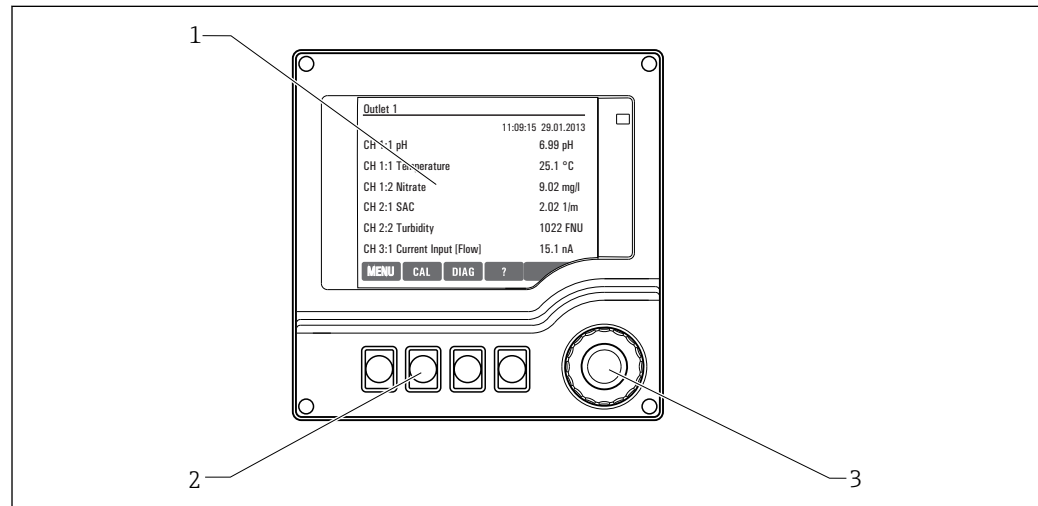

A0025231


36 Overview of operation

- 1 Display (with red display background in alarm condition)
- 2 Soft keys (function depends on menu)
- 3 Navigator (jog/shuttle and press/hold function)



Remote operation

Via HART (e.g. using HART modem and FieldCare)

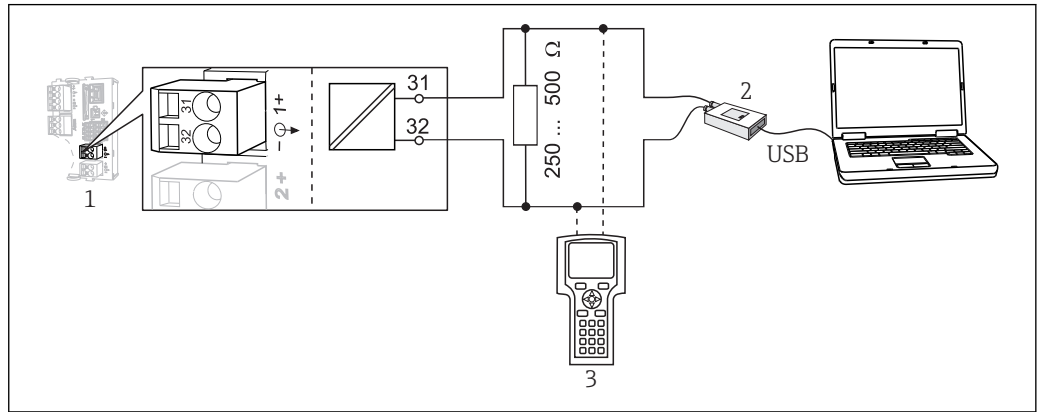


A0028995

37 HART using modem

- 1 Device module Base L, H or E: current output 1 with HART
  - 2 HART modem for connection to PC, e.g. Commubox FXA191 (RS232) or FXA195 <sup>1)</sup> (USB)
  - 3 HART handheld terminal
- 1) Switch position "on" (substitutes the resistor)


Via PROFIBUS DP

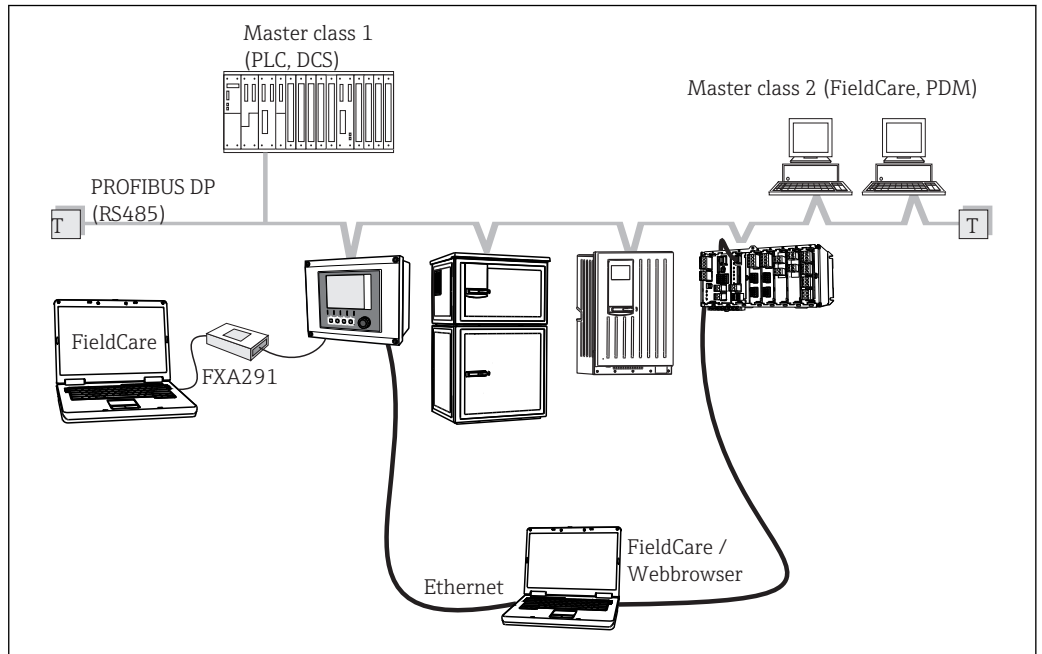

A0028991

38 PROFIBUS DP


T Terminating resistor

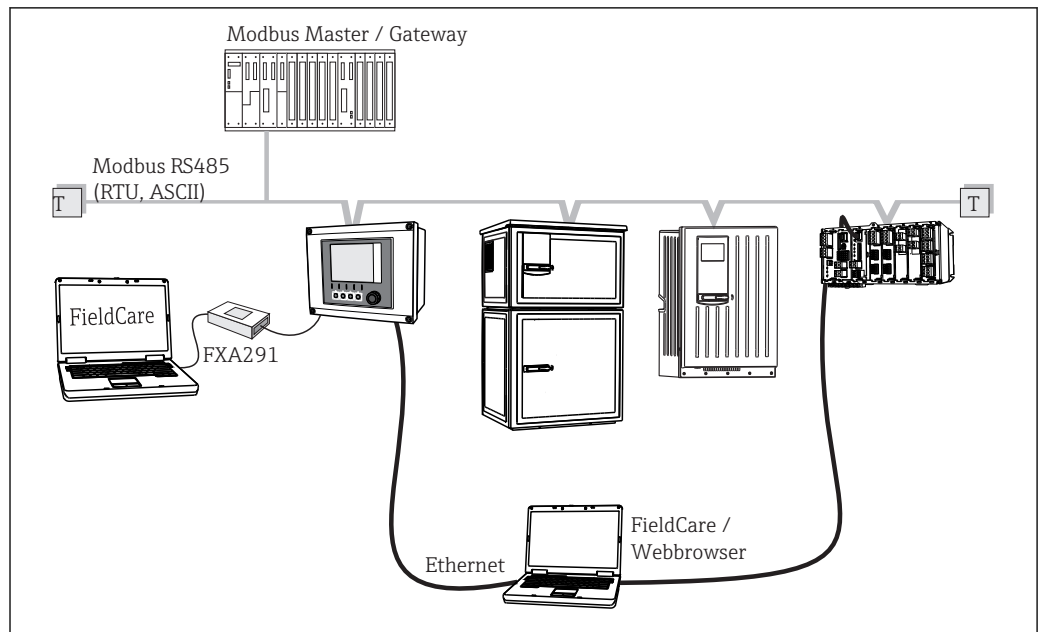**Via Modbus RS485**

A0028993

39 Modbus RS485

T Terminating resistor

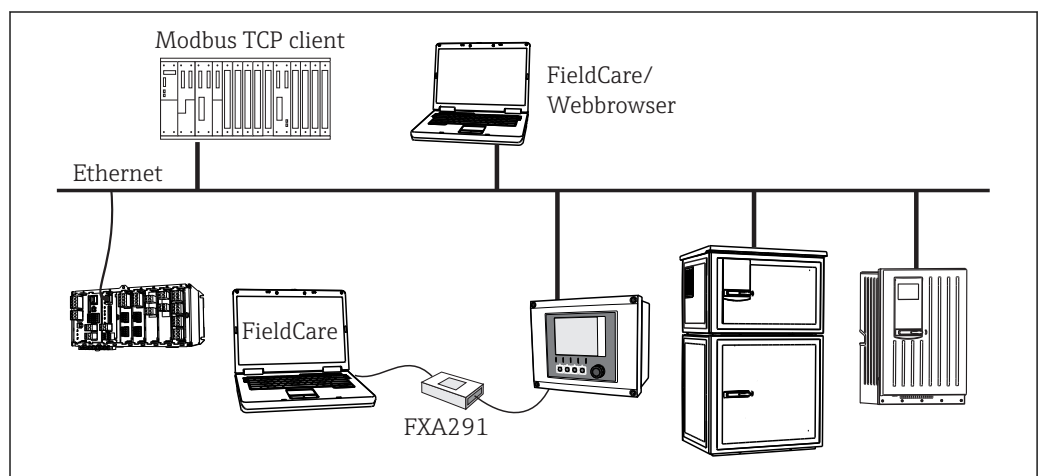**Via Ethernet/Web server/Modbus TCP/EtherNet/IP**

A0028994

40 Modbus TCP and/or EtherNet/IP

**Language packages**

The language selected in the product structure is the operating language preset at the factory. All other languages can be selected using the menu.

- English (US)
- German
- Chinese (Simplified, PR China)
- Czech
- Dutch
- French
- Italian
- Japanese
- Polish
- Portuguese
- Russian
- Spanish
- Swedish

- Turkish
- Hungarian
- Croatian
- Vietnamese

The availability of other languages can be checked via the product structure at [www.endress.com/cm442R](http://www.endress.com/cm442R) or [.../cm444R](http://www.endress.com/cm444R) or [.../cm448R](http://www.endress.com/cm448R).


## Certificates and approvals

<b>CE mark</b>	The product meets the requirements of the harmonized European standards. As such, it complies with the legal specifications of the EU directives. The manufacturer confirms successful testing of the product by affixing to it the <b>CE</b> mark.
<b>EAC</b>	The product has been certified according to guidelines TP TC 004/2011 and TP TC 020/2011 which apply in the European Economic Area (EEA). The EAC conformity mark is affixed to the product.
<b>cCSAus</b>	<p>The device has been certified with regard to its electrical safety and for NI Class I Div. 2 cCSAus explosion-proof environments. It meets the requirements in accordance with:</p> <ul style="list-style-type: none"> <li>▪ CLASS 2252 06 - Process Control Equipment</li> <li>▪ CLASS 2252 86 - Process Control Equipment - Certified to US Standards</li> <li>▪ CLASS 2258 03 - Process Control Equipment - Intrinsically Safe and Non-incendive Systems - For Hazardous Locations</li> <li>▪ CLASS 2258 83 - Process Control Equipment - Intrinsically Safe and Non-incendive Systems - For Hazardous Locations - Certified to US Standards</li> <li>▪ FM3600</li> <li>▪ FM3611</li> <li>▪ FM3810</li> <li>▪ ANSI/ISA NEMA250</li> <li>▪ IEC 60529</li> <li>▪ CAN/CSA-C22.2 No. 0</li> <li>▪ CAN/CSA C22.2 No. 94</li> <li>▪ CSA Std. C22.2 No. 213</li> <li>▪ CAN/CSA-C22.2 No. 61010-1</li> <li>▪ CAN/CSA-C22.2 No. 60529</li> <li>▪ UL/ANSI/ISA 61010-1</li> <li>▪ ANSI - ISA 12 12 01</li> </ul> <p>► The device must be installed in a housing or cabinet where access is only possible with a tool or key.</p>

## Ordering information

<b>Product page</b>	<p><a href="http://www.endress.com/cm442r">www.endress.com/cm442r</a></p> <p><a href="http://www.endress.com/cm444r">www.endress.com/cm444r</a></p> <p><a href="http://www.endress.com/cm448r">www.endress.com/cm448r</a></p>
<b>Product Configurator</b>	<p>On the product page there is a <b>Configure</b> button to the right of the product image.</p> <ol style="list-style-type: none"> <li>1. Click this button. <ul style="list-style-type: none"> <li>↳ The Configurator opens in a separate window.</li> </ul> </li> <li>2. Select all the options to configure the device in line with your requirements. <ul style="list-style-type: none"> <li>↳ In this way, you receive a valid and complete order code for the device.</li> </ul> </li> </ol>

3. Export the order code as a PDF or Excel file. To do so, click the appropriate button on the right above the selection window.

 For many products you also have the option of downloading CAD or 2D drawings of the selected product version. Click the **CAD** tab for this and select the desired file type using picklists.

#### Scope of delivery

The scope of delivery comprises:

- 1 multichannel controller in the version ordered
- 1 mounting plate
- 1 external display (if selected as an option) <sup>2)</sup>
- 1 DIN rail power unit incl. Cable (CM444R and CM448R only)
- 1 printed copy of the Operating Instructions for DIN rail power unit
- 1 printed copy of the Brief Operating Instructions in the language ordered

## Accessories

The following are the most important accessories available at the time this documentation was issued.

- ▶ For accessories not listed here, please contact your Service or Sales Center.

#### Measuring cable

##### Memosens data cable CYK10

- For digital sensors with Memosens technology
- Product Configurator on the product page: [www.endress.com/cyk10](http://www.endress.com/cyk10)



Technical Information TI00118C

##### Memosens data cable CYK11

- Extension cable for digital sensors with Memosens protocol
- Product Configurator on the product page: [www.endress.com/cyk11](http://www.endress.com/cyk11)



Technical Information TI00118C

#### Sensors

##### Glass electrodes

###### Orbisint CPS11D

- pH sensor for process technology
- Optional SIL version for connecting to SIL transmitter
- With dirt-repellent PTFE diaphragm
- Product Configurator on the product page: [www.endress.com/cps11d](http://www.endress.com/cps11d)



Technical Information TI00028C

###### Memosens CPS31D

- pH electrode with gel-filled reference system with ceramic diaphragm
- Product Configurator on the product page: [www.endress.com/cps31d](http://www.endress.com/cps31d)



Technical Information TI00030C

###### Ceraliquid CPS41D

- pH electrode with ceramic junction and KCl liquid electrolyte
- Product Configurator on the product page: [www.endress.com/cps41d](http://www.endress.com/cps41d)



Technical Information TI00079C

###### Ceragel CPS71D

- pH electrode with reference system including ion trap
- Product Configurator on the product page: [www.endress.com/cps71d](http://www.endress.com/cps71d)



Technical Information TI00245C

2) The external display can be selected as an option in the order structure or ordered as an accessory at a later stage.

#### **Memosens CPS171D**

- pH electrode for bio-fermenters with digital Memosens technology
- Product Configurator on the product page: [www.endress.com/cps171d](http://www.endress.com/cps171d)



Technical Information TI01254C

#### **Orbipore CPS91D**

- pH electrode with open aperture for media with high dirt load
- Product Configurator on the product page: [www.endress.com/cps91d](http://www.endress.com/cps91d)



Technical Information TI00375C

#### **Orbipac CPF81D**

- Compact pH sensor for installation or immersion operation
- In industrial water and wastewater
- Product Configurator on the product page: [www.endress.com/cpf81d](http://www.endress.com/cpf81d)



Technical Information TI00191C

#### **Enamel pH electrodes**

##### **Ceramax CPS341D**

- pH electrode with pH-sensitive enamel
- Meets highest demands of measuring accuracy, pressure, temperature, sterility and durability
- Product Configurator on the product page: [www.endress.com/cps341d](http://www.endress.com/cps341d)



Technical Information TI00468C

#### **ORP sensors**

##### **Orbisint CPS12D**

- ORP sensor for process technology
- Product Configurator on the product page: [www.endress.com/cps12d](http://www.endress.com/cps12d)



Technical Information TI00367C

##### **Ceraliquid CPS42D**

- ORP electrode with ceramic junction and KCl liquid electrolyte
- Product Configurator on the product page: [www.endress.com/cps42d](http://www.endress.com/cps42d)



Technical Information TI00373C

##### **Ceragel CPS72D**

- ORP electrode with reference system including ion trap
- Product Configurator on the product page: [www.endress.com/cps72d](http://www.endress.com/cps72d)



Technical Information TI00374C

##### **Orbipac CPF82D**

- Compact ORP sensor for installation or immersion operation in process water and wastewater
- Product Configurator on the product page: [www.endress.com/cpf82d](http://www.endress.com/cpf82d)



Technical Information TI00191C

##### **Orbipore CPS92D**

- ORP electrode with open aperture for media with high dirt load
- Product Configurator on the product page: [www.endress.com/cps92d](http://www.endress.com/cps92d)



Technical Information TI00435C

#### **pH ISFET sensors**

##### **Tophit CPS441D**

- Sterilizable ISFET sensor for low-conductivity media
- Liquid KCl electrolyte
- Product Configurator on the product page: [www.endress.com/cps441d](http://www.endress.com/cps441d)



Technical Information TI00352C

**Tophit CPS471D**

- Sterilizable and autoclavable ISFET sensor for food and pharmaceuticals, process engineering
- Water treatment and biotechnology
- Product Configurator on the product page: [www.endress.com/cps471d](http://www.endress.com/cps471d)



Technical Information TI00283C

**Tophit CPS491D**

- ISFET sensor with open aperture for media with high dirt load
- Product Configurator on the product page: [www.endress.com/cps491d](http://www.endress.com/cps491d)



Technical Information TI00377C

**pH and ORP combined sensors****Memosens CPS16D**

- Combined pH/ORP sensor for process technology
- With dirt-repellent PTFE diaphragm
- With Memosens technology
- Product Configurator on the product page: [www.endress.com/cps16D](http://www.endress.com/cps16D)



Technical Information TI00503C

**Memosens CPS76D**

- Combined pH/ORP sensor for process technology
- Hygienic and sterile applications
- With Memosens technology
- Product Configurator on the product page: [www.endress.com/cps76d](http://www.endress.com/cps76d)



Technical Information TI00506C

**Memosens CPS96D**

- Combined pH/ORP sensor for chemical processes
- With poison-resistant reference with ion trap
- With Memosens technology
- Product Configurator on the product page: [www.endress.com/cps96d](http://www.endress.com/cps96d)



Technical Information TI00507C

**Conductivity sensors with inductive measurement of conductivity****Indumax CLS50D**

- High-durability inductive conductivity sensor
- For standard and hazardous area applications
- With Memosens technology
- Product Configurator on the product page: [www.endress.com/cls50d](http://www.endress.com/cls50d)



Technical Information TI00182C

**Indumax H CLS54D**

- Inductive conductivity sensor
- With certified, hygienic design for foodstuffs, beverages, pharmaceuticals and biotechnology
- Product Configurator on the product page: [www.endress.com/cls54d](http://www.endress.com/cls54d)



Technical Information TI00508C

**Conductivity sensors with conductive measurement of conductivity****Condumax CLS15D**

- Conductive conductivity sensor
- For pure water, ultrapure water and hazardous area applications
- Product Configurator on the product page: [www.endress.com/CLS15d](http://www.endress.com/CLS15d)



Technical Information TI00109C

#### **Condumax CLS16D**

- Hygienic, conductive conductivity sensor
- For pure water, ultrapure water and Ex applications
- With EHEDG and 3A approval
- Product Configurator on the product page: [www.endress.com/CLS16d](http://www.endress.com/CLS16d)



Technical Information TI00227C

#### **Condumax CLS21D**

- Two-electrode sensor in plug-in head version version
- Product Configurator on the product page: [www.endress.com/CLS21d](http://www.endress.com/CLS21d)



Technical Information TI00085C

#### **Memosens CLS82D**

- Four-electrode sensor
- With Memosens technology
- Product Configurator on the product page: [www.endress.com/cls82d](http://www.endress.com/cls82d)



Technical Information TI01188C

#### **Oxygen sensors**

##### **Oxymax COS22D**

- Sterilizable sensor for dissolved oxygen
- With Memosens technology or as an analog sensor
- Product Configurator on the product page: [www.endress.com/cos22d](http://www.endress.com/cos22d)



Technical Information TI00446C

##### **Oxymax COS51D**

- Amperometric sensor for dissolved oxygen
- With Memosens technology
- Product Configurator on the product page: [www.endress.com/cos51d](http://www.endress.com/cos51d)



Technical Information TI00413C

##### **Oxymax COS61D**

- Optical oxygen sensor for drinking water and industrial water measurement
- Measuring principle: quenching
- With Memosens technology
- Product Configurator on the product page: [www.endress.com/cos61d](http://www.endress.com/cos61d)



Technical Information TI00387C

##### **Memosens COS81D**

- Sterilizable, optical sensor for dissolved oxygen
- With Memosens technology
- Product Configurator on the product page: [www.endress.com/cos81d](http://www.endress.com/cos81d)



Technical Information TI01201C

#### **Disinfection sensors**

##### **CCS142D**

- Membrane-covered amperometric sensor for free chlorine
- Measuring range 0.01 to 20 mg/l
- With Memosens technology
- Product Configurator on the product page: [www.endress.com/ccs142d](http://www.endress.com/ccs142d)



Technical Information TI00419C

**Ion-selective sensors****ISEmax CAS40D**

- Ion selective sensors
- Product Configurator on the product page: [www.endress.com/cas40d](http://www.endress.com/cas40d)



Technical Information TI00491C

**Turbidity sensors****Turbimax CUS51D**

- For nephelometric measurements of turbidity and solids in wastewater
- 4-beam scattered light method
- With Memosens technology
- Product Configurator on the product page: [www.endress.com/cus51d](http://www.endress.com/cus51d)



Technical Information TI00461C

**Turbimax CUS52D**

- Hygienic Memosens sensor for turbidity measurement in drinking water, process water and in utilities
- With Memosens technology
- Product Configurator on the product page: [www.endress.com/cus52d](http://www.endress.com/cus52d)



Technical Information TI01136C

**SAC and nitrate sensors****Viomax CAS51D**

- SAC and nitrate measurement in drinking water and wastewater
- With Memosens technology
- Product Configurator on the product page: [www.endress.com/cas51d](http://www.endress.com/cas51d)



Technical Information TI00459C

**Interface measurement****Turbimax CUS71D**

- Immersion sensor for interface measurement
- Ultrasonic interface sensor
- Product Configurator on the product page: [www.endress.com/cus71d](http://www.endress.com/cus71d)



Technical Information TI00490C

**Additional functionality****Hardware extension modules****Kit, extension module AOR**

- 2 x relay, 2 x 0/4 to 20 mA analog output
- Order No. 71111053

**Kit, extension module 2R**

- 2 x relay
- Order No. 71125375

**Kit, extension module 4R**

- 4 x relay
- Order No. 71125376

**Kit, extension module 2AO**

- 2 x 0/4 to 20 mA analog output
- Order No. 71135632

**Kit, extension module 4AO**

- 4 x analog output 0/4 to 20 mA
- Order No. 71135633

**Kit, extension module 2DS**

- 2 x digital sensor, Memosens
- Order No. 71135631



**Kit, extension module 2AI**

- 2 x 0/4 to 20 mA analog input
- Order No. 71135639

**Kit, extension module DIO**

- 2 x digital input
- 2 x digital output
- Auxiliary voltage supply for digital output
- Order No. 71135638

**Kit, extension module 485**

- Ethernet configuration
- Can be extended to PROFIBUS DP or Modbus RS485 or Modbus TCP or EtherNet/IP. This requires an additional activation code which can be ordered separately.
- Order No. 71135634

**Kit, extension module ETH**

- Ethernet configuration
- Can be extended to Modbus TCP or EtherNet/IP. This requires an additional activation code which can be ordered separately.
- Order No. 71279810

**Upgrade kit, extension module 485 with PROFIBUS DP**

- Extension module 485
- PROFIBUS DP (+ Ethernet configuration)
- Order No. 71140888

**Upgrade kit, extension module 485 with Modbus RS485**

- Extension module 485
- Modbus RS485 (+ Ethernet configuration)
- Order No. 71140889

**Upgrade kit, extension module 485 with Modbus TCP**

- Extension module 485
- Modbus TCP (+ Ethernet configuration)
- Order No. 71140890

**Upgrade kit, extension module 485 with EtherNet/IP**

- Extension module 485
- EtherNet/IP (+ Ethernet configuration)
- Order No. 71219868

**Upgrade kit, extension module ETH with Modbus TCP**

- Extension module ETH
- Modbus TCP (+ Ethernet configuration)
- Order No. 71279809

**Upgrade kit, extension module ETH with EtherNet/IP**

- Extension module ETH
- EtherNet/IP (+ Ethernet configuration)
- Order No. 71279812

**Firmware and activation codes**

**SD card with Liquiline firmware**

- Industrial Flash Drive, 1 GB
- Order No. 71127100



You must quote the serial number of the device when ordering the activation code.

**Activation code for digital HART communication**

Order No. 71128428

**Activation code for PROFIBUS DP**

Order No. 71135635

**Activation code for Modbus RS485**

Order No. 71135636

**Activation code for Modbus TCP for module 485**

Order No. 71135637

**Activation code for EtherNet/IP for module 485**

Order No. 71219871

**Activation code for Modbus TCP for module ETH**

Order No. 71279813

**Activation code for EtherNet/IP for module ETH**

Order No. 71279830

**Kit CM442R: activation code for 2nd digital sensor input**

Order No. 71114663

**Kit CM444R/CM448R: upgrade code for 2 x 0/4 to 20 mA for BASE-E**

Order No. 71140891

**Activation code for feedforward control**

- Requires current input or fieldbus communication
- Order No. 71211288

**Activation code for measuring range switch**

- Requires digital inputs or fieldbus communication
- Order No. 71211289

**Activation code for ChemocleanPlus**

- Requires relays or digital outputs or fieldbus communication and optional digital inputs
- Order No. 71239104

**Activation code for Heartbeat Verification and Monitoring**

Order No. 71367524

**Activation code for ion exchanger operating time**

- Mathematical function
- Order No. 71367531

**Activation code for mathematics**

- Formula editor
- Order No. 71367541

**Activation code for remote calibration interface**

Order No. 71367542

**Software****Memobase Plus CYZ71D**

- PC software to support laboratory calibration
- Visualization and documentation of sensor management
- Sensor calibrations stored in database
- Product Configurator on the product page: [www.endress.com/cyz71d](http://www.endress.com/cyz71d)



Technical Information TI00502C

**Field Data Manager Software MS20**

- PC software for central data management
- Visualization of series of measurements and logbook events
- SQL database for secure data storage

**Other accessories****External display<sup>3)</sup>****Graphic display**

- For installation in the control cabinet door or panel
- Order No. 71185295

**Service display**

- Portable, for commissioning
- Order No. 71185296

**SD card**

- Industrial Flash Drive, 1 GB
- Weight: 2 g
- Order No. 71110815

<sup>3)</sup> The external display can be selected as an option in the product structure or ordered subsequently as an accessory.

### Communication-specific accessories

#### Commubox FXA191

- Intrinsically safe HART communication with FieldCare via the RS232C interface
- Transforms HART signals on RS 232C interface



Technical Information TI00237F

#### Commubox FXA195

Intrinsically safe HART communication with FieldCare via the USB port



Technical Information TI00404F

#### Commubox FXA291

Connects the CDI interface of measuring devices with the USB port of the computer or laptop



Technical Information TI00405C

#### Wireless HART adapter SWA70

- Wireless device connection
- Easily integrated, offers data protection and transmission safety, can be operated in parallel with other wireless networks, minimum cabling complexity



Technical Information TI00061S

#### Fieldgate FXA320

Gateway for the remote interrogation of 4-20 mA measuring devices via a Web browser



Technical Information TI00025S

#### FieldXpert SFX100

Compact, flexible and robust industrial handheld terminal for remote configuration and for obtaining measured values via the HART current output



Operating Instructions BA00060S

### System components

#### RIA14, RIA16

- Field display unit for integration into 4-20 mA circuits
- RIA14 in flameproof metal enclosure



Technical Information TI00143R and TI00144R

#### RIA15

- Process display unit, Digital display unit for integration into 4-20 mA circuits
- Panel mounting
- With optional HART communication



Technical Information TI01043K

[www.addresses.endress.com](http://www.addresses.endress.com)

---