

# Technical Information

## Liquiline M CM42

Memosens: pH/ORP, oxygen, conductivity

Analog sensors: pH/ORP, conductivity, concentration, resistivity



### Two-wire transmitter for Ex and non-Ex areas

#### Application

Liquiline M CM42 is a modular two-wire transmitter for all areas of process engineering.

Depending on the version ordered, Liquiline has one or two analog current outputs. In addition, it can be connected to fieldbuses in accordance with the FOUNDATION Fieldbus, PROFIBUS PA and HART protocol.

The transmitter is suitable for pollution degree 3.

The highly robust plastic version and the hygienic stainless steel version are tailored to the following applications:

- Chemical processes
- Pharmaceuticals industry
- Foodstuff technology
- Applications in hazardous areas

#### Your benefits

- Cost-saving:
  - Simple commissioning with Quick Setup and Navigator
  - Memosens: Plug & play laboratory-calibrated sensors
  - Predictive maintenance system detects when a sensor needs to be cleaned, calibrated or replaced.
  - Less storage thanks to modular design
  - Effective asset management using FieldCare and W@M
- Safe:
  - Memosens: Active display of cable interruption
  - User-guided commissioning, graphic display and plain text guidance for maximum operating safety
  - Approvals: ATEX, FM, CSA, NEPSI, TIIS
  - User administration: Code-protected commissioning
  - pH glass with Memosens: SIL2 measuring point with TÜV approval

## Table of contents


|  |           |   |           |
|--|-----------|---|-----------|
| <b>Function and system design</b> .....                    | <b>3</b>  | <b>Installation</b> .....               | <b>25</b> |
| Measuring system .....                                     | 3         | Wall securing plate .....               | 25        |
| <b>Equipment architecture</b> .....                        | <b>4</b>  | Weather protection cover .....          | 25        |
| Software .....   | 4         | Installation options .....              | 26        |
| DAT memory modules .....                                   | 5         | Installation in Ex area .....           | 27        |
| Suitable sensors .....                                     | 5         | <b>Environment</b> .....                | <b>29</b> |
| <b>Dependability</b> .....                                 | <b>5</b>  | Ambient temperature range .....         | 29        |
| Reliability .....  | 5         | Storage temperature .....               | 29        |
| Maintainability .....                                      | 7         | Electromagnetic compatibility .....     | 29        |
| Safety .....   | 7         | Degree of protection .....              | 29        |
| <b>Input</b> .....   | <b>8</b>  | Relative humidity .....                 | 29        |
| Measured variables .....                                   | 8         | Pollution degree .....                  | 29        |
| Measuring ranges .....                                     | 8         | <b>Mechanical construction</b> .....    | <b>29</b> |
| Binary input (Memosens): pH/ORP, oxygen, conductivity .... | 8         | Dimensions .....                        | 29        |
| Analog input: pH / ORP .....                               | 9         | Weight .....                            | 30        |
| Analog input: Conductivity .....                           | 10        | Material .....                          | 30        |
| <b>Output</b> .....  | <b>11</b> | <b>Operability</b> .....                | <b>31</b> |
| Output signal .....  | 11        | Operation concept .....                 | 31        |
| Signal on alarm .....                                      | 11        | Display characteristics .....           | 31        |
| Load .....   | 11        | Operating elements .....                | 31        |
| Output signal range .....                                  | 11        | <b>Ordering information</b> .....       | <b>32</b> |
| Ex specification current output .....                      | 11        | Product page .....                      | 32        |
| Ex specification PROFIBUS and FOUNDATION Fieldbus ....     | 12        | Product configurator .....              | 32        |
| <b>Protocol-specific data</b> .....                        | <b>12</b> | Scope of delivery .....                 | 32        |
| HART .....   | 12        | <b>Certificates and approvals</b> ..... | <b>32</b> |
| PROFIBUS PA .....  | 12        | CE mark .....                           | 32        |
| FOUNDATION Fieldbus .....                                  | 12        | Ex approval .....                       | 32        |
| <b>Current output, passive</b> .....                       | <b>13</b> | <b>Accessories</b> .....                | <b>33</b> |
| Span .....   | 13        | Mounting kits .....                     | 33        |
| Signal characteristics .....                               | 13        | Weather protection cover .....          | 33        |
| Cable specification .....                                  | 13        | Active barrier .....                    | 33        |
| <b>Power supply</b> .....                                  | <b>13</b> | Fieldbus accessories .....              | 33        |
| Supply voltage .....                                       | 13        | Measuring cable .....                   | 34        |
| Cable specification .....                                  | 13        | Sensors .....                           | 34        |
| Grounding the housing .....                                | 14        | Software update and upgrade .....       | 37        |
| Supply and signal voltage .....                            | 15        |   |           |
| Sensor connection .....                                    | 17        |   |           |
| Sensor connection: Memosens sensors .....                  | 18        |   |           |
| Sensor connection: analog pH/ORP sensors .....             | 19        |   |           |
| Sensor connection: analog conductivity sensors .....       | 23        |   |           |
| <b>Performance characteristics</b> .....                   | <b>24</b> |   |           |
| Reference temperature .....                                | 24        |   |           |
| Current output response time .....                         | 24        |   |           |
| Memosens measured error .....                              | 24        |   |           |
| Tolerance, current outputs .....                           | 24        |   |           |
| Repeatability .....  | 24        |   |           |
| Temperature compensation conductivity .....                | 24        |   |           |
| Temperature adjustment .....                               | 25        |   |           |

## Function and system design

### Measuring system

A complete measuring system consists of:

- Liquiline M CM42 transmitter with mounting plate (e.g. for wall mounting)
- sensor and suitable sensor cable
- assembly suitable for the sensor (optional)
- post retainer (optional)
- weather protection cover (optional)

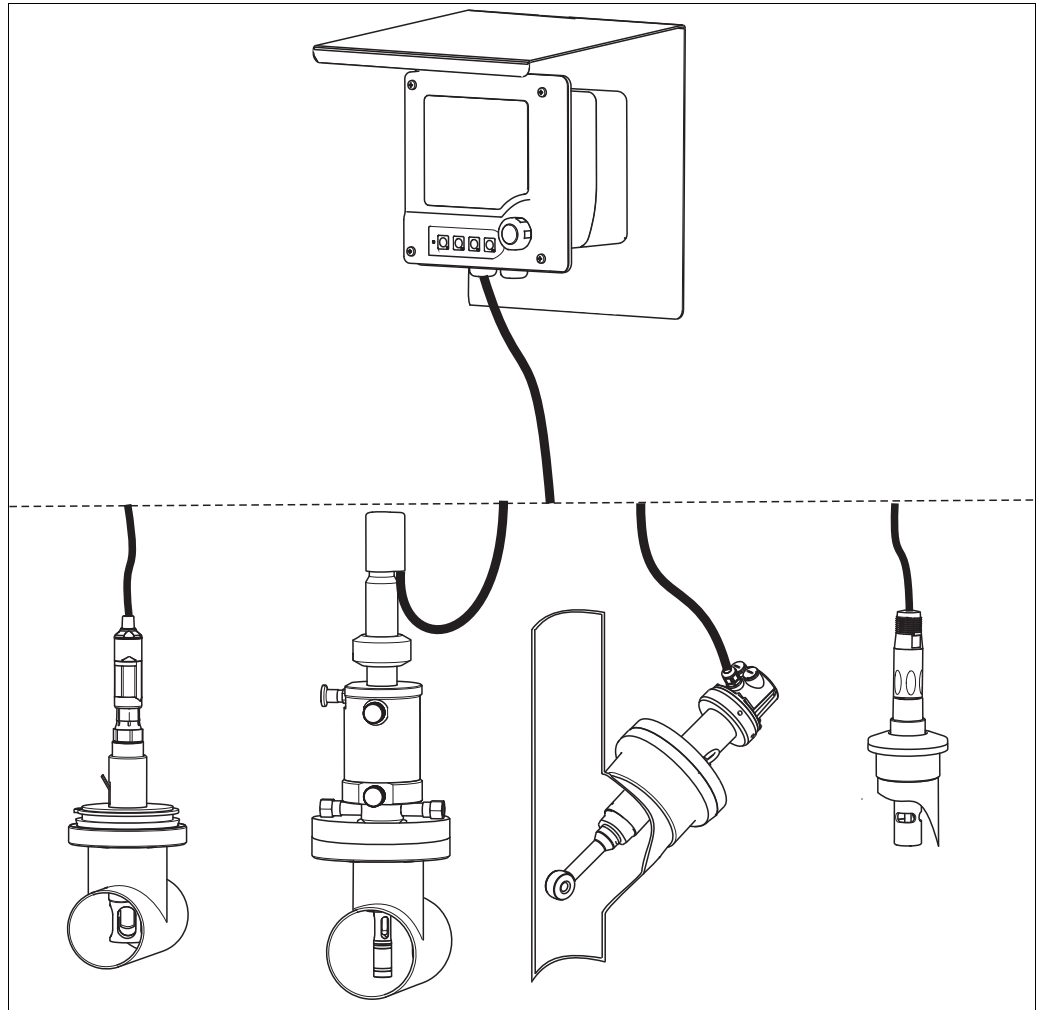

Examples of a measuring system

#### pH / ORP (analog)

- CM42-P...
- Measuring cable CPK9
- Cleanfit CPA471 assembly
- Orbisint CPS11 sensor

#### Conductivity, inductive measurement (analog)

- CM42-I...
- Dipfit CLA111 assembly
- Indumax CLS50 sensor

#### Conductivity, conductive measurement (analog)

- CM42-C...
- Measuring cable CPK9
- Condumax CLS16 sensor

#### Memosens (digital)

- CM42-K/L/M/N/O...
- Measuring cable CYK10
- (Unifit CPA442 assembly)
- Sensor <sup>1)</sup>

<sup>1)</sup> CPS11D (pH glass), CPS471D (pH ISFET), CPS16D (pH/ORP combined), CPS341D (enamel pH), COS22D/COS51D (DO), CLS15D/CLS16D/CLS21D (LFc), CLS50D (LFi)

You can combine your measuring point with a range of assemblies and sensors. Details can be found in the "Accessories" section and in the documentation listed there. For additional information, see [www.endress.com/cm42](http://www.endress.com/cm42)

#### NOTICE

##### Effect of climatic conditions: rain, snow, direct sun

Impaired operation to complete transmitter failure

- ▶ When installing outside, always use the weather protection cover (see accessories).

## Equipment architecture

### Software

You can choose from the following software packages:

- Standard:  
Standard application for the most common measuring points
- Advanced:  
Many additional functions that increase safety and quality

| Package   | Features  |  |   |   |  |   |
|---|---|--|---|---|--|---|
|   | pH /ORP (glass/ISFET)   | Conductivity   | Oxygen  |   |  |   |
| <b>Standard</b>   | <p><b>Analog sensors</b></p> <ul style="list-style-type: none"> <li>- Offset and two-point calibration</li> <li>- Sample calibration</li> <li>- Calibration with standard buffers</li> <li>- Manual buffer specification</li> <li>- Temperature compensation</li> <li>- Temperature adjustment</li> <li>- Isotherm intersection</li> <li>- Simulation of current output</li> <li>- Self-diagnosis</li> <li>- Calibration stability settings</li> <li>- Clock</li> </ul> <p><b>Memosens sensors</b><br/>as for analog with the addition of:</p> <ul style="list-style-type: none"> <li>- Sensor information</li> <li>- Sensor check</li> </ul>   | <p><b>Analog sensors</b></p> <ul style="list-style-type: none"> <li>- Sample calibration</li> <li>- Temperature calibration: one-point</li> <li>- Temperature compensation: linear, NaCl, ultrapure water (NaCl, HCl)</li> <li>- Simulation of current output</li> <li>- Self-diagnosis</li> <li>- Concentration measurement</li> <li>- Clock</li> </ul> <p><b>Memosens sensors</b><br/>as for analog with the addition of:</p> <ul style="list-style-type: none"> <li>- Sensor information</li> <li>- Sensor check</li> </ul> | <p><b>Memosens sensors</b></p> <ul style="list-style-type: none"> <li>- Slope calibration                             <ul style="list-style-type: none"> <li>- in air (100% rF)</li> <li>- in water (100% air-saturated)</li> </ul> </li> <li>- in air (with input of current absolute air pressure and relative humidity)</li> <li>- Zero point calibration</li> <li>- Sample calibration</li> <li>- Temperature adjustment</li> <li>- Medium compensation</li> <li>- Calibration stability settings</li> <li>- Simulation of current output</li> <li>- Self-diagnosis</li> <li>- Clock</li> <li>- Sensor information</li> <li>- Sensor check</li> </ul> |   |  |   |
| <b>Advanced</b>   | <p><b>"Standard" software package with the addition of:</b></p> <table border="0" style="width: 100%;"> <tr> <td style="vertical-align: top; width: 33%;"> <p><b>Analog sensors</b></p> <ul style="list-style-type: none"> <li>- Medium compensation</li> <li>- Calibration timer</li> <li>- Sensor Condition Check (SCC)</li> <li>- Process Check System (PCS)</li> </ul> <p><b>Memosens sensors</b><br/>as for analog with the addition of:</p> <ul style="list-style-type: none"> <li>- Operated hours counter</li> <li>- Sterilization cnt.</li> </ul> </td> <td style="vertical-align: top; width: 33%;"> <p><b>Analog sensors</b></p> <ul style="list-style-type: none"> <li>- Calibration with separate installation factor (inductive measurement only)</li> <li>- Polarization detection (conductive measurement only)</li> <li>- Temperature compensation via user table</li> <li>- Two-point temperature adjustment: offset and slope</li> <li>- USP alarm and prealarm</li> </ul> <p><b>Memosens sensors</b><br/>as for analog with the addition of:</p> <ul style="list-style-type: none"> <li>- Operated hours counter</li> <li>- Sterilization cnt.</li> </ul> </td> <td style="vertical-align: top; width: 33%;"> <p><b>Memosens sensors</b></p> <ul style="list-style-type: none"> <li>- Polarization voltage setting</li> <li>- Calibration timer</li> <li>- Sensor statistics</li> <li>- Operated hours counter</li> <li>- Sterilization cnt.</li> </ul> </td> </tr> </table> <p>All devices, regardless of measurement parameter</p> <ul style="list-style-type: none"> <li>- Logbooks</li> <li>- Data logbook</li> <li>- Free assignment of measured values to current outputs (optional)</li> <li>- Switching on and off of diagnostic function</li> <li>- Extended user administration</li> <li>- Current output tables</li> </ul> |  |   | <p><b>Analog sensors</b></p> <ul style="list-style-type: none"> <li>- Medium compensation</li> <li>- Calibration timer</li> <li>- Sensor Condition Check (SCC)</li> <li>- Process Check System (PCS)</li> </ul> <p><b>Memosens sensors</b><br/>as for analog with the addition of:</p> <ul style="list-style-type: none"> <li>- Operated hours counter</li> <li>- Sterilization cnt.</li> </ul> | <p><b>Analog sensors</b></p> <ul style="list-style-type: none"> <li>- Calibration with separate installation factor (inductive measurement only)</li> <li>- Polarization detection (conductive measurement only)</li> <li>- Temperature compensation via user table</li> <li>- Two-point temperature adjustment: offset and slope</li> <li>- USP alarm and prealarm</li> </ul> <p><b>Memosens sensors</b><br/>as for analog with the addition of:</p> <ul style="list-style-type: none"> <li>- Operated hours counter</li> <li>- Sterilization cnt.</li> </ul> | <p><b>Memosens sensors</b></p> <ul style="list-style-type: none"> <li>- Polarization voltage setting</li> <li>- Calibration timer</li> <li>- Sensor statistics</li> <li>- Operated hours counter</li> <li>- Sterilization cnt.</li> </ul> |
| <p><b>Analog sensors</b></p> <ul style="list-style-type: none"> <li>- Medium compensation</li> <li>- Calibration timer</li> <li>- Sensor Condition Check (SCC)</li> <li>- Process Check System (PCS)</li> </ul> <p><b>Memosens sensors</b><br/>as for analog with the addition of:</p> <ul style="list-style-type: none"> <li>- Operated hours counter</li> <li>- Sterilization cnt.</li> </ul> | <p><b>Analog sensors</b></p> <ul style="list-style-type: none"> <li>- Calibration with separate installation factor (inductive measurement only)</li> <li>- Polarization detection (conductive measurement only)</li> <li>- Temperature compensation via user table</li> <li>- Two-point temperature adjustment: offset and slope</li> <li>- USP alarm and prealarm</li> </ul> <p><b>Memosens sensors</b><br/>as for analog with the addition of:</p> <ul style="list-style-type: none"> <li>- Operated hours counter</li> <li>- Sterilization cnt.</li> </ul>  | <p><b>Memosens sensors</b></p> <ul style="list-style-type: none"> <li>- Polarization voltage setting</li> <li>- Calibration timer</li> <li>- Sensor statistics</li> <li>- Operated hours counter</li> <li>- Sterilization cnt.</li> </ul>  |   |   |  |   |

## DAT memory modules

There are 3 different types of DAT module, which can be ordered as an optional accessory or are already included in the scope of delivery:

- **SystemDAT**  
Firmware updates (newer firmware version) or change of language pack
- **FunctionDAT**  
Extended functional range ("Advanced" firmware or second current output)
- **CopyDAT**  
Memory for own configuration settings

### Test the extensibility of your device

- ▶ Before ordering a FunctionDAT, check if it is possible to extend the functional range of your device.
- 

## Suitable sensors

### pH/ORP

- Analog and Memosens glass electrodes
- Analog and Memosens ISFET sensors
- Analog and Memosens ORP sensors
- Memosens pH/ORP combined sensors
- Analog and Memosens enamel pH electrodes
- Analog single electrodes (glass or antimony)

### Conductivity

- Analog and Memosens, conductive sensors
  - Two-electrode sensors
  - Four-electrode sensors
- Analog and Memosens, inductive sensors

### Oxygen

Amperometric sensors:

- with Memosens technology
  - 12 and 40 mm design
- 

# Dependability

---

## Reliability

### Memosens



Memosens makes your measuring point safer:

- No-contact, digital signal transmission allows optimum galvanic isolation
- No contact corrosion
- Completely watertight
- Sensors can be calibrated in a lab, which increases the availability of measured values
- Predictive maintenance thanks to recording of sensor data, e.g.:
  - Total hours of operation
  - Hours of operation with very high or very low measured values
  - Operating hours at high temperatures
  - Number of steam sterilizations
  - Sensor status

### Quick Setup


#### To the first measured value within 1 minute

Once you have set up the few parameters in the Quick Setup menu, the measuring point is ready to measure. The first measured value is reliably displayed.

---

### Process Check System (PCS): Life check

This function is used to check the measuring signal for stagnation. An alarm is triggered if the measuring signal does not change over a certain period (several measured values). The reason for such behavior can be contamination, clogging or similar.

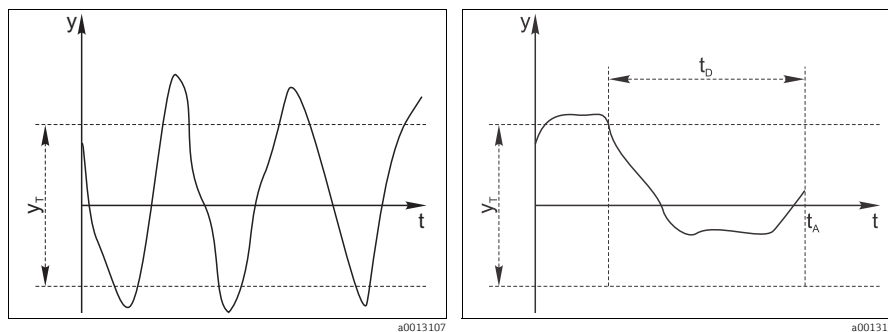

Normal measuring signal, no alarm

$y$  Measuring signal  
 $y_T$  Minimum signal fluctuation

Stagnating signal, alarm is triggered

$t_D$  Specified time interval  
 $t_A$  Time at which the alarm is triggered

### Sensor Condition Check (SCC, pH only)

This function monitors the electrode status and the degree of electrode aging. The status is displayed with the messages "SCC electrode condition bad" or "SCC electrode condition sufficient". The status of the electrode is updated after every calibration.

### Sensor Check System (SCS, pH only)

The Sensor Check System monitors the pH glass resistance or reference resistance (for analog and combined sensors only), thus indicating possible incorrect measurements that may occur as a result of damage to or clogging of the pH electrode.

In addition, the SCS detects glass breakage in the case of classic glass electrodes as well as leaks in the case of ISFET sensors.

### Polarization monitoring (conductivity only, conductively measured)

Polarization effects in the boundary layer between the sensor and the measuring solution limit the measuring range of conductive conductivity sensors.

The transmitter can detect and report polarization effects using an intelligent signal evaluation process.

### United States Pharmacopeia, USP and European Pharmacopeia, EP (conductivity only)

The requirements for ultrapure water in the pharmaceutical industry are determined primarily by the American USP and European EP.

The transmitter complies with USP/EP requirements for conductivity measuring systems:

- Exact temperature measurement at the place of conductivity measurement
- Simultaneous display of uncompensated conductivity values and temperature is possible
- Display resolution 0.01  $\mu\text{S}/\text{cm}$
- Exact factory calibration of the transmitter with traceable precision resistance (optional)
- Exact adjustment of sensors in the factory as per ASTM D 1125-91 or ASTM D 5391-99 (optional)
- Temperature-dependent measured value monitoring as per USP and EP.

The limit functions for pharmaceutical water are implemented in the "Advanced" software package in accordance with USP and EP: For conductivity measurements, the limit functions for pharmaceutical water are implemented in the software in accordance with USP and EP:

- Water for Injection (WFI) as per USP <645> and EP
- Highly purified water (HPW) as per EP
- Purified water (PW) as per EP

The uncompensated conductivity value and the temperature are measured for the USP/EP limit functions. The measured values are compared with the tables set down in the standards. An alarm is triggered if the limit value is exceeded. In addition, a prealarm can be set that flags undesirable operating statuses before they occur.

**Application-optimized calibration models (oxygen)**

In separate functions, the transmitter allows process-adjusted zero point sensor calibration or sensor calibration via the slope.


There are different calibration models for this, ranging from simple slope calibration in air that is saturated with water vapor to slope calibration with input of the absolute air pressure and relative humidity at the measuring location.

The latter model allows in-process calibration during operation as well as during sterilization and cleaning.

The number of calibrations and sterilizations are tracked separately for the sensor and membrane cap. The relevant counter can be reset if the membrane cap is replaced.

**Maintainability**

**Modular design**

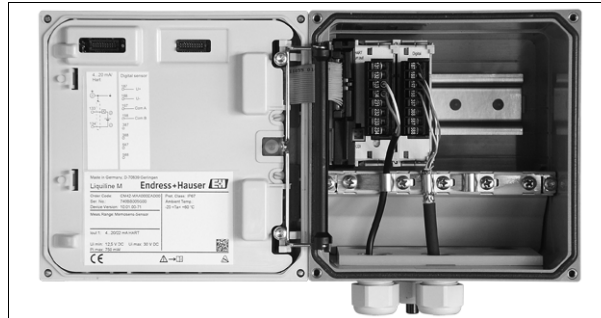

a0010477

Interior of Liquiline (version with sensor module)




a0010476

Plug-in modules


**Sensor monitor ("Advanced" only)**

You will find the sensor monitor in the DIAG menu. Important sensor data incl. warning and alarm limits are displayed either graphically or numerically.

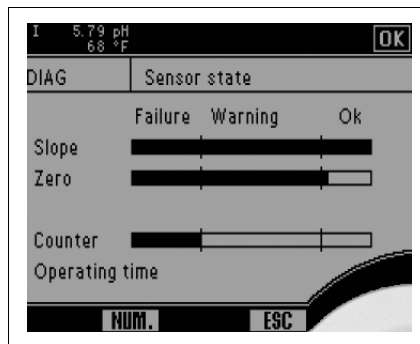

a0010474

Sensor monitor, graphical display (example)

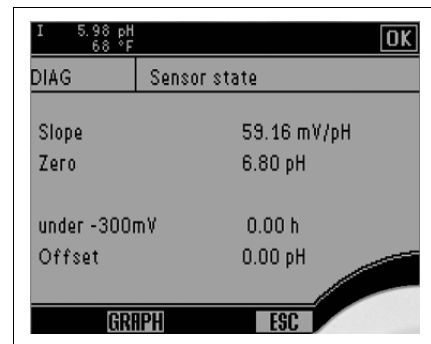

a0014566

Sensor monitor, numerical display (example)

**Safety**

**User administration ("Advanced" only)**

To avoid unscheduled changes to the measuring point, the device features a user administration function.

You need to log on as an Expert to switch on the user administration function. The first time you log onto the device, you will therefore be asked to enter a password (the "Admin" user name is already entered).

The user administration function makes two different modes available in the Advanced version:

**Roles**

- There are 3 fixed user roles (Expert, Maintenance, Operator).
- "Experts" always have all the rights. "Operator" is the role with the least amount of rights.
- Each role has its own individual password. This password can be changed.
- No other user roles can be created.

**User accounts**

- You can create and manage a maximum of 15 user accounts.
- You need to be logged on as an "Expert" to be able to manage accounts.
- In each user account you specify the user name and the password and assign the new user one of 3 user roles (Operator, Maintenance and Expert).
- Multiple user accounts with the "Expert" role are possible.

**SIL**

A TÜV-approved SIL2 version of the Liquiline M CM42 is also available (CM42-M\* only, without HART).

**Safety functions**

- Safe output of the digitized value at the current output
- Monitoring of the measured value for leaving a defined interval
- Safe calibration and adjustment

**i** Additional information and Safety Manuals can be found at:  
[www.endress.com/SIL](http://www.endress.com/SIL)



## Input

**Measured variables** --> Documentation of the connected sensor

**Measuring ranges** --> Documentation of the connected sensor

**Binary input (Memosens):**  
 pH/ORP, oxygen,  
 conductivity



**Cable specification**

|  |                                  |
|--|----------------------------------|
| CYK10, CYK20 with Memosens                 | Max. cable length 100 m (330 ft) |
| Fixed cable with Memosens (CLS50D, CLS54D) | Max. cable length 100 m (330 ft) |

**Ex specification**

|   |        |
|---|--------|
| Intrinsically safe sensor circuit with protection type: Ex ia IIC <sup>1)</sup> or Ex ic IIC <sup>2)</sup> or Ex ib IIC <sup>3)</sup> |        |
| Max. output voltage U <sub>o</sub>  | 5.04 V |
| Max. output current I <sub>o</sub>  | 80 mA  |
| Max. output P <sub>o</sub>  | 112 mW |
| Max. external inductance L <sub>o</sub>   | 2 µH   |
| Max. external capacitance C <sub>o</sub>  | 55 µF  |

- 1) CM42-\*G\*\*\*\*\*, CM42-\*E\*\*\*\*\*, CM42-\*I\*\*\*\*\*, CM42-\*J\*\*\*\*\*,  
 CM42-\*X\*\*\*\*\*, CM42-\*Z\*\*\*\*\*
- 2) CM42-\*V\*\*\*\*\*, CM42-\*F\*\*\*\*\*
- 3) CM42-\*T\*\*\*\*\*



**Analog input: pH / ORP****Cable specification**

|             |                                 |
|-------------|---------------------------------|
| Without SCS | Max. cable length 50 m (160 ft) |
| With SCS    | Max. cable length 20 m (65 ft)  |

**Applicable temperature sensors**

- Pt100
- Pt1000
- NTC 30K

**Ex specification**

|  |              |              |
|--|--------------|--------------|
| Intrinsically safe sensor circuit with protection type: Ex ia IIC <sup>1)</sup> or Ex ic IIC <sup>2)</sup> |              |              |
|  | <b>Glass</b> | <b>ISFET</b> |
| Max. output voltage $U_o$  | 10.08 V      | 10.08 V      |
| Max. output current $I_o$  | 4.1 mA       | 50.7 mA      |
| Max. output $P_o$  | 10.2 mW      | 128 mW       |
| Max. external inductance $L_o$   | 1 mH         | 1 mH         |
| Max. external capacitance $C_o$  | 250 nF       | 250 nF       |
| Connection class as per NE116 <sup>3)</sup>  | SensISCO1X   | -            |

- 1) CM42-\*G\*\*\*\*\* , CM42-\*E\*\*\*\*\* , CM42-\*I\*\*\*\*\* , CM42-\*X\*\*\*\*\* , CM42-\*Z\*\*\*\*\*
- 2) CM42-\*V\*\*\*\*\* , CM42-\*F\*\*\*\*\*
- 3) CM42-\*G\*\*\*\*\* , CM42-\*E\*\*\*\*\* , CM42-\*F\*\*\*\*\*

When pH/ORP glass electrodes are connected to terminals 317, 318, 320, 111, 112 and 113, the device corresponds to connection class 1 as per NAMUR Recommendation NE116 (SensISCO). Terminals 315 and 316 may not be connected for this categorization. The device is labeled SensISCO1X.

**Input impedance**

>  $1 \cdot 10^{12} \Omega$  (under nominal operating conditions)

**Input leakage current**

<  $1 \cdot 10^{-13} \text{ A}$  (under nominal operating conditions)

## Analog input: Conductivity

## Cable specification

|   |   |
|---|---|
| Conductivity/specific resistivity, conductively measured <sup>1)</sup><br>Two-electrode sensor<br>10 $\mu\text{S}\cdot\text{k}$ to 20 $\text{mS}\cdot\text{k}$ / 0.1 $\text{M}\Omega/\text{k}$ to 50 $\Omega/\text{k}$<br>5 $\mu\text{S}\cdot\text{k}$ to 20 $\text{mS}\cdot\text{k}$ / 0.2 $\text{M}\Omega/\text{k}$ to 50 $\Omega/\text{k}$<br>0.1 $\mu\text{S}\cdot\text{k}$ to 20 $\text{mS}\cdot\text{k}$ / 20 $\text{M}\Omega/\text{k}$ to 50 $\Omega/\text{k}$ | Max. cable length 100 m (330 ft)<br>Max. cable length 50 m (160 ft)<br>Max. cable length 15 m (50 ft) |
| Conductivity, measured conductively<br>Four-electrode sensor<br>10 $\mu\text{S}\cdot\text{k}$ to 1.5 $\text{S}\cdot\text{k}$<br>0.1 $\mu\text{S}\cdot\text{k}$ to 20 $\text{mS}\cdot\text{k}$   | Max. cable length 100 m (330 ft)<br>Max. cable length 15 m (50 ft)                                    |
| Conductivity, measured inductively <sup>2)</sup>  | max. cable length 55 m (180 ft) (CLS50)<br>max. cable length 50 m (160 ft) (CLS54)                    |

1) with cable CYK71, CPK9 or fixed cable

2) with cable CLK5, CLK6 or fixed cable

## Applicable temperature sensors

- Pt100
- Pt1000

## Ex specification, conductive sensors

|  |                   |
|--|-------------------|
| Intrinsically safe sensor circuit with protection type: Ex ia IIC <sup>1)</sup> or Ex ic IIC <sup>2)</sup> |                   |
| Max. output voltage $U_o$  | 10.08 V           |
| Max. output current $I_o$  | 23 mA             |
| Max. output $P_o$  | 57 mW             |
| Max. external inductance $L_o$   | 300 $\mu\text{H}$ |
| Max. external capacitance $C_o$  | 50 nF             |

1) CM42-\*G\*\*\*\*\* , CM42-\*E\*\*\*\*\* , CM42-\*I\*\*\*\*\* , CM42-\*X\*\*\*\*\* , CM42-\*Z\*\*\*\*\*

2) CM42-\*V\*\*\*\*\* , CM42-\*F\*\*\*\*\*

## Ex specification, inductive sensors

|   |                   |
|---|-------------------|
| Intrinsically safe sensor circuit with protection type: Ex ia IIC <sup>1)</sup> or Ex ic IIC <sup>2)</sup> or Ex ib IIC <sup>3)</sup> |                   |
| Max. output voltage $U_o$   | 10.08 V           |
| Max. output current $I_o$   | 64 mA             |
| Max. output $P_o$   | 128 mW            |
| Max. external inductance $L_o$  | 0.1 mH            |
| Max. external conductivity $C_o$  | 1.8 $\mu\text{F}$ |

1) CM42-\*G\*\*\*\*\* , CM42-\*E\*\*\*\*\* , CM42-\*I\*\*\*\*\* , CM42-\*J\*\*\*\*\* , CM42-\*X\*\*\*\*\* , CM42-\*Z\*\*\*\*\*

2) CM42-\*V\*\*\*\*\* , CM42-\*F\*\*\*\*\*

3) CM42-\*T\*\*\*\*\*

## Output

### Output signal

#### Current output

1x 4 to 20 mA, passive, potentially isolated against sensor circuit (Memosens only)<sup>1)2)</sup>  
 2x 4 to 20 mA, passive, potentially isolated against sensor circuit (Memosens only) and against each other<sup>1)2)3)</sup>

#### HART

|                               |                                 |
|-------------------------------|---------------------------------|
| Signal coding                 | FSK ± 0.5 mA via current signal |
| Data transmission rate        | 1200 Baud                       |
| Load (communication resistor) | 250 Ω                           |

#### PROFIBUS PA

|                                   |   |
|-----------------------------------|---|
| Signal coding                     | Manchester Coding Bus Powered (MBP), compliant with IEC 61158-2 |
| Data transmission rate            | 31.25 kBit/s  |
| Bus termination                   | external  |
| Connection to PROFIBUS-DP network | via segment coupler (in non-Ex mode)                            |

#### FOUNDATION Fieldbus

|                        |   |
|------------------------|---|
| Signal coding          | Manchester Coding Bus Powered (MBP), compliant with IEC 61158-2 |
| Data transmission rate | 31.25 kBit/s  |
| Bus termination        | external  |

### Signal on alarm

3.6 to 21.5 mA (4.0 mA fixed value in HART multidrop mode)  
 digitally via fieldbus<sup>4)</sup>

### Load

Max. load with supply voltage of 24 V: 500 Ω  
 Max. load with supply voltage of 30 V: 750 Ω

### Output signal range

3.6 to 21.5 mA

### Ex specification current output

|  |   |
|--|---|
| Intrinsically safe supply and signal circuits, passive |   |
| Max. input voltage $U_i$                               | 30 V                                      |
| Max. input current $I_i$                               | 100 mA                                    |
| Max. input $P_i$                                       | 800 mW (all except TIIS) or 750 mW (TIIS) |
| Max. internal inductance $L_i$                         | 29 μH (output 1)<br>24 μH (output 2)      |
| Max. internal capacitance $C_i$                        | 1.2 nF (output 1)<br>0.2 nF (output 2)    |

- 1) Potential isolation for Memosens in sensor plug
- 2) For inductive sensors with Memosens protocol CLS50D and CLS54D not potentially isolated against sensor circuit!
- 3) Current output 1 and current output 2 (optional)
- 4) For version with PROFIBUS PA or FOUNDATION Fieldbus

**Ex specification PROFIBUS  
and FOUNDATION Fieldbus**

|   |             |
|---|-------------|
| Suitable for use as a field device in a FISCO system as per EN/IEC 60079-27 |             |
| Max. input voltage $U_i$  | 17.5 V      |
| Max. input current $I_i$  | 380 mA      |
| Max. input $P_i$  | 5.32 W      |
| Max. internal inductance $L_i$  | <10 $\mu$ H |
| Max. internal capacitance $C_i$   | < 5 nF      |

**Protocol-specific data****HART**

|                                   |  |
|-----------------------------------|--|
| Manufacturer ID                   | 11 <sub>h</sub>  |
| Device type                       | 11A0 <sub>h</sub> (CM42-M/N/P), 11A1 <sub>h</sub> (CM42-C/I/K/L), 11A1 <sub>h</sub> (CM42-O)       |
| Device revision                   | 001 <sub>h</sub>   |
| Device description files (DD/DTM) | www.endress.com<br>Device Integration Manager (DIM)  |
| Device variables                  | 7 (CM42-M/N/O/P), 3 (CM42-C/I/K/L), pre-defined device variables, dynamic variables PV, SV, TV, QV |
| Supported features                | PDM DD, AMS DD, DTM, handheld DDs  |

**PROFIBUS PA**

|                    |  |
|--------------------|--|
| Manufacturer ID    | 11 <sub>h</sub>  |
| Device type        | 1565 <sub>h</sub> (CM42-M/N/P), 1566 <sub>h</sub> (CM42-C/I/K/L), 1567 <sub>h</sub> (CM42-O)<br>in compatibility mode<br>1543 <sub>h</sub> (CM42-M/N/P), 1544 <sub>h</sub> (CM42-C/I/K/L), 1545 <sub>h</sub> (CM42-O), 9750 <sub>h</sub> (profile identifier, analyzer PA devices)   |
| Profile version    | PA Profile 3.02  |
| GSD files          | www.endress.com/profibus<br>Device Integration Manager DIM   |
| Output variables   | 6 AI blocks  |
| Supported features | <ul style="list-style-type: none"> <li>▪ 1 MSCY0 connection (cyclical communication, master class 1 to slave)</li> <li>▪ 1 MSAC1 connection (acyclical communication, master class 1 to slave)</li> <li>▪ 2 MSAC2 connections (acyclical communication, master class 2 to slave)</li> <li>▪ Addressing with DIL switches or via software</li> <li>▪ GSD, PDM DD, DTM</li> <li>▪ Status output: condensed or classic</li> </ul> |

**FOUNDATION Fieldbus**

|                            |   |
|----------------------------|---|
| Manufacturer name:         | Endress+Hauser                                      |
| Model name:                | Liquiline_Cond                                      |
| Manufacturer ID (hex):     | 452B48  |
| Device type (hex):         | 10A1  |
| Device revision (hex):     | 2   |
| Device class:              | Link master   |
| ITK version:               | 6.1.1   |
| Function and other blocks: | 1xRB, 6xAI, 2xDI, 1xPID, 2xAALM, 1xISEL, 1xSC, 7xTB |


## Current output, passive

|                               |  |
|-------------------------------|--|
| <b>Span</b>                   | 3.6 to 21.5 mA                               |
| <b>Signal characteristics</b> | linear, table ("Advanced" only)              |
| <b>Cable specification</b>    | Cable type: shielded wire, Ø 2.5 mm (14 AWG) |

## Power supply

### Supply voltage

Current output / HART:

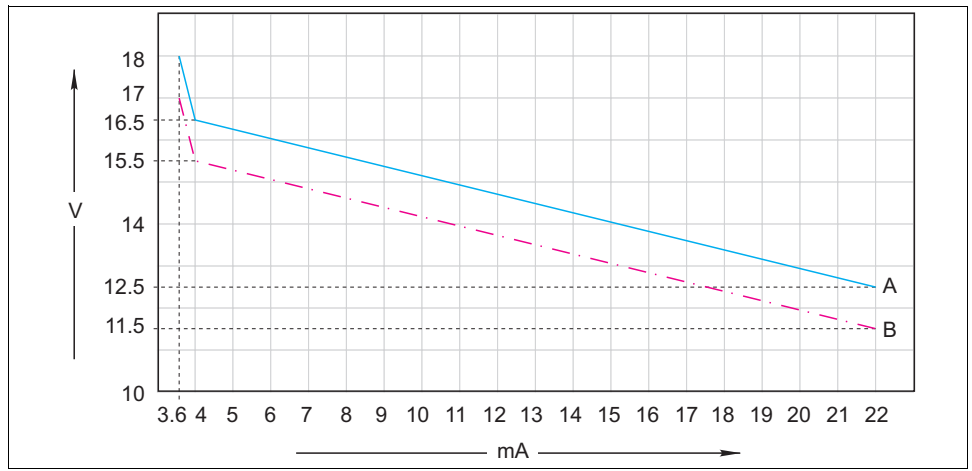

Minimum supply voltage at the transmitter depending on the output current

A with HART communication  
B without HART communication

|                                    |  |
|------------------------------------|--|
| PROFIBUS PA / FOUNDATION Fieldbus: | 9 to 32 V DC (non-Ex)<br>9 to 17.5 V DC (Ex) |
| Bus current consumption:           | 22 mA  |

### Cable specification

### Certified cable glands

| Cable gland    | Clamping range, permitted cable diameter |
|----------------|--|
| M16 x 1.5 mm   | 3 to 6 mm (0.12 to 0.24")                |
| M20 x 1.5 mm   | 5 to 9 mm (0.20 to 0.35")                |
| M20 x 1.5 mm   | 6 to 12 mm (0.24 to 0.47")               |
| NPT 3/8"       | 3 to 6 mm (0.12 to 0.24")                |
| NPT 1/2"       | 5 to 9 mm (0.20 to 0.35")                |
| NPT 1/2"       | 6 to 12 mm (0.24 to 0.47")               |
| G3/8           | 3 to 6 mm (0.12 to 0.24")                |
| G1/2           | 5 to 9 mm (0.20 to 0.35")                |
| G1/2           | 9 to 12 mm (0.35 to 0.47")               |
| Dummy plug M16 | -  |
| Dummy plug M20 | -  |


**Cable cross-section**

max. cable cross-section: 2.5 mm<sup>2</sup> (i14 AWG), GND 4 mm<sup>2</sup> (i12 AWG)

**Grounding the housing****Plastic housing****⚠ WARNING****Electric voltage at ungrounded cable mounting rail**

No shock protection

- ▶ Connect the cable mounting rail to the foundation ground using a separate  $\geq 2.5 \text{ mm}^2$  (14 AWG) functional ground.

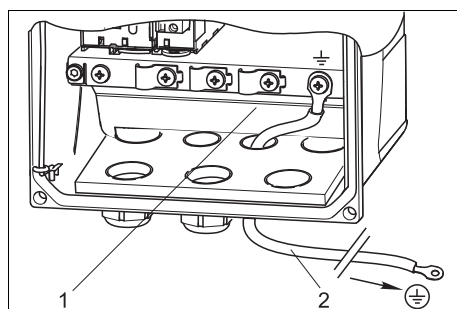


Grounding the housing

- 1 Cable mounting rail  
2  $\geq 2.5 \text{ mm}^2$  (14 AWG) functional ground

**Stainless steel housing****⚠ WARNING****Electric voltage at ungrounded housing**

No shock protection

- ▶ Connect the external ground connection of the housing to the foundation ground using a separate wire (GN/YE) ( $\geq 2.5 \text{ mm}^2$ , corresponds to 14 AWG).

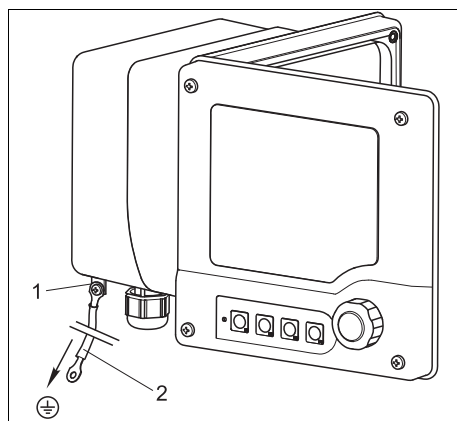

Grounding the housing

- 1 Outer ground connection  
2  $\geq 2.5 \text{ mm}^2$  (14 AWG) wire (GN/YE)


Supply and signal voltage

4 to 20 mA

- ▶ Connect the transmitter with a shielded two-wire cable.
  - ↳ How the shield is connected depends on the interference influence expected. To suppress electrical fields, it suffices to ground the shield at one end. If you also want to suppress interference from a magnetic alternating field, you must ground the shield at both ends.

In the case of a SIL device, you must ground both current outputs at both ends.


**i** The second current output can be ordered as an option (see "Ordering information").

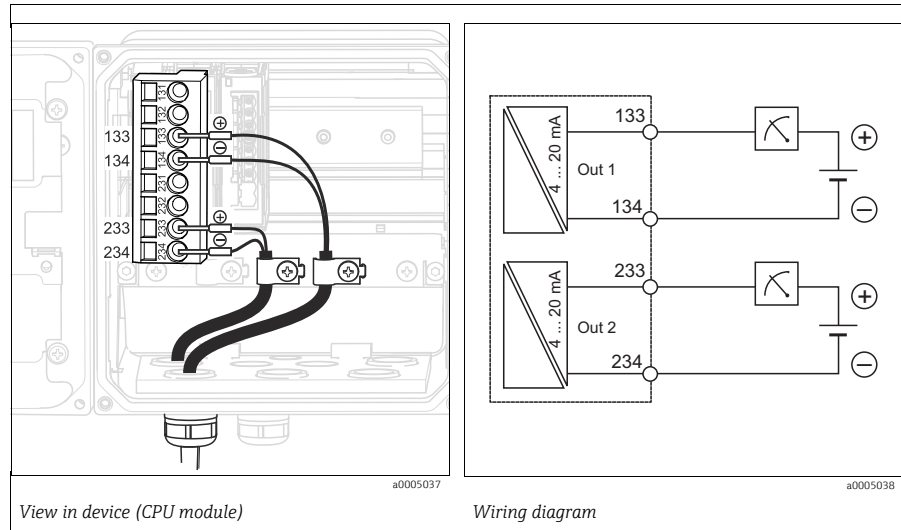

4 to 20 mA / HART

For safe communication via the HART protocol and for compliance with NAMUR NE 21, you must use a two-wire cable that is grounded at both ends.

- ▶ Connect the transmitter to a two-wire cable that is grounded at both ends.

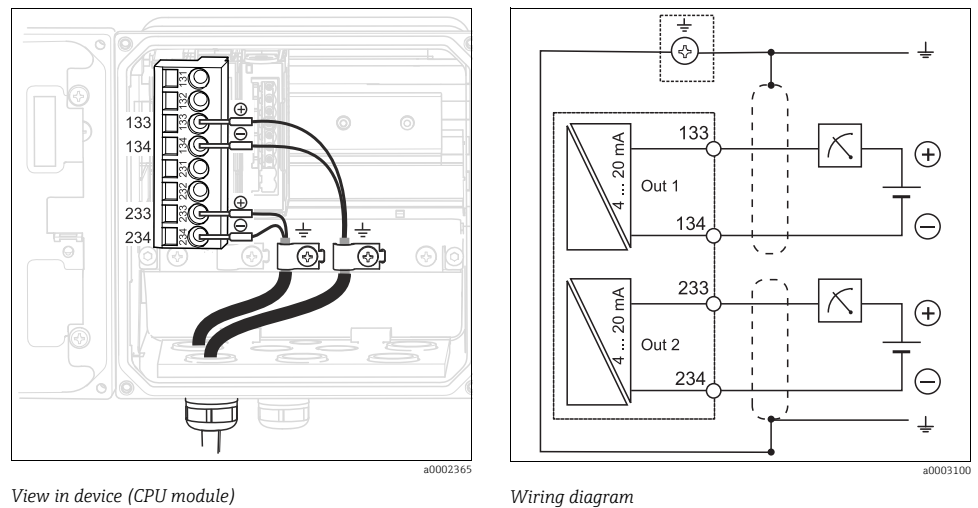

**i** The device is powered only via current output 1 and not via current output 2.

### PROFIBUS PA and FOUNDATION Fieldbus


Use a fieldbus cable grounded at both ends (device **and** PCS).

There are various ways of connecting the unit:


1. Two-wire cable grounded at both ends, "hard grounding" (generally to be given priority over "capacitive connection to ground")
2. If there is a risk of large potential equalization currents. Shielded two-wire cabling, "capacitive connection to ground" (shield grounded on device side via capacitor, "C-module" accessory required)  
**Do not use in the hazardous area!**
3. Use the fieldbus connection socket (accessories)

#### "Hard grounding"

1. Connect the cable shield to the cable mounting rail.
2. Connect the cable cores as per the assignment.

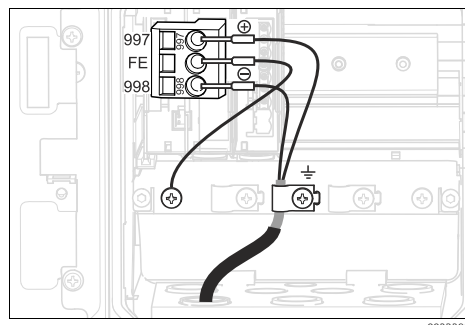


View in device (CPU module)

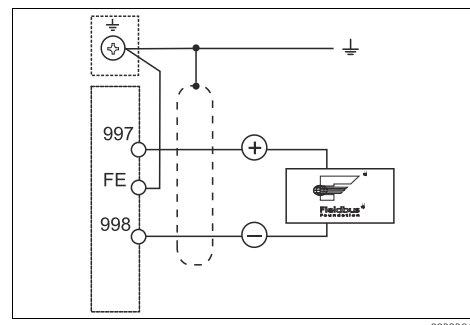


Wiring diagram

#### "Capacitive ground connection"


1. Pull back the braided shield, put the stranded extension wire of the C-module (item 1) onto the exposed shield and tighten the clip:

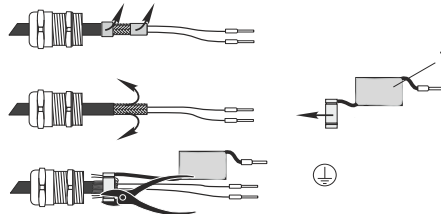

2. Connect the extension wire to the cable mounting rail.
3. Connect the cable cores as per the assignment.

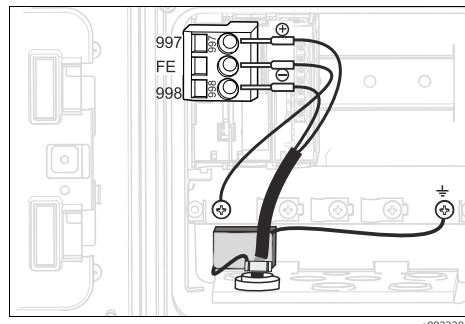

View in device (CPU module)

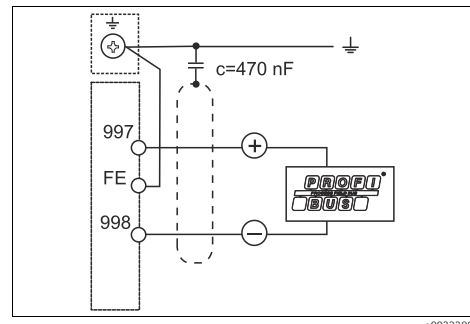


Wiring diagram




**"Fieldbus connection socket"**

1. Screw the fieldbus connection socket into the housing bushing.
2. Trim the connection cores of the socket to approx. 15 cm.
3. Connect the cable cores as per the assignment. In doing so, you must connect the cable shield (GN/YE) to the cable mounting rail.

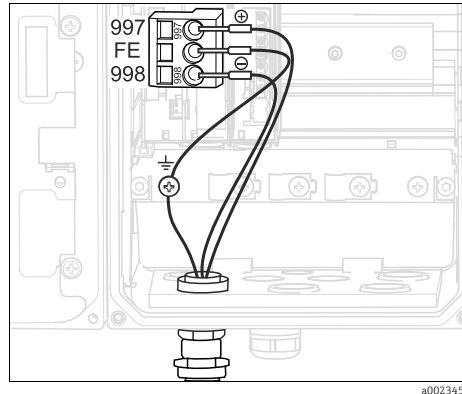

View in device (CPU module)

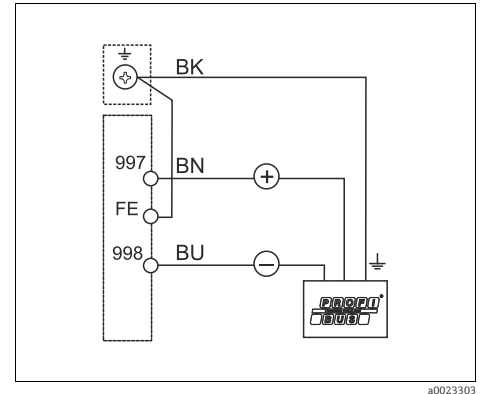

Wiring diagram

**Sensor connection**

| Explanation of abbreviations in the following diagrams: |   |
|---|---|
| Abbreviation  | Meaning                                     |
| pH  | pH signal                                   |
| Ref   | Signal from reference electrode             |
| Src   | Source                                      |
| Drn   | Drain                                       |
| PM  | Potential matching                          |
| U <sub>+</sub>  | Power supply of the digital sensor          |
| U <sub>-</sub>  |   |
| Com A   | Communication signals of the digital sensor |
| Com B   |   |
| ϑ   | Signal of the temperature sensor            |
| d.n.c.  | Do not connect!                             |


**NOTICE****No shielding against electrical and magnetic interference**

Interference can give erroneous measurement results

- ▶ You must connect shielded connections or terminals with functional earth ( $\perp$ ) (there is no protective earth in the case of the plastic housing ( $\oplus$ )).
- ▶ Keep magnetic interference fields away from the sensor since inductive conductivity sensors use magnetic fields.


Sensor connection:  
Memosens sensors

pH/ORP incl. pH/ORP combined sensors, oxygen, conductively measured conductivity

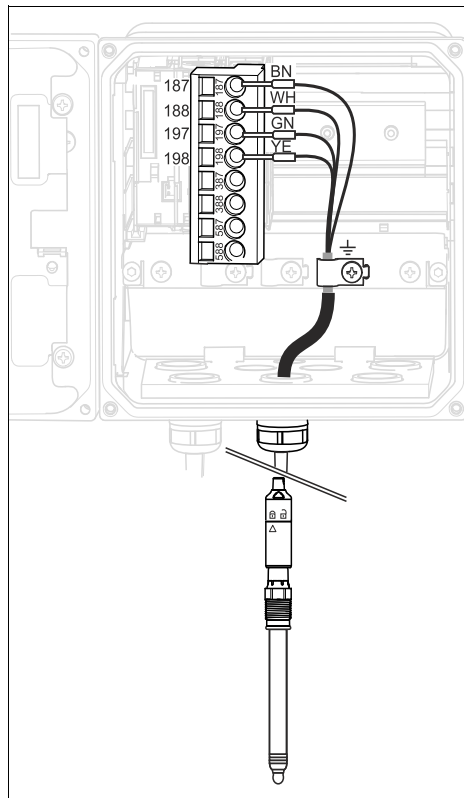

View in device (sensor module)


a0001087

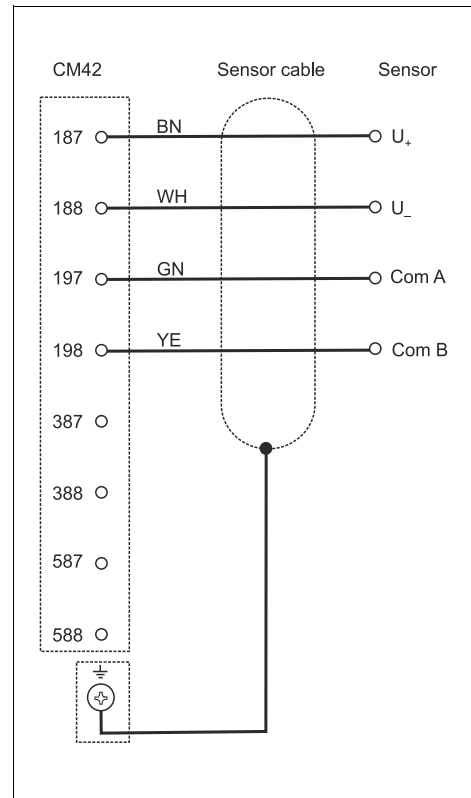

Wiring diagram


a0001078

inductively measured conductivity

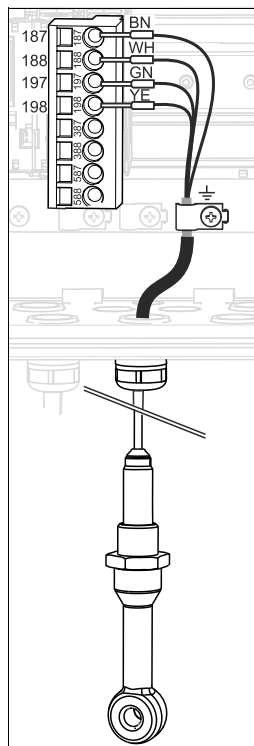

View inside device

a0014525

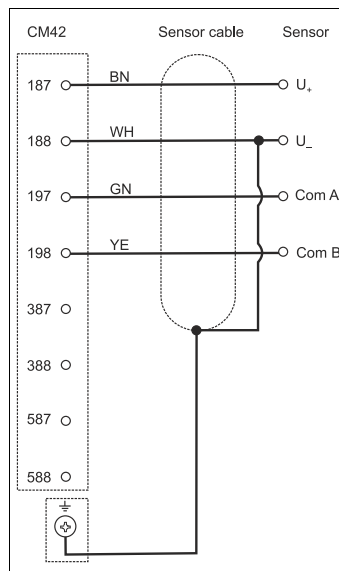


Wiring diagram

CLS50D to serial numbers J2xxxx05LI0

CLS54D to serial numbers H8xxxx05LI1

a0020732

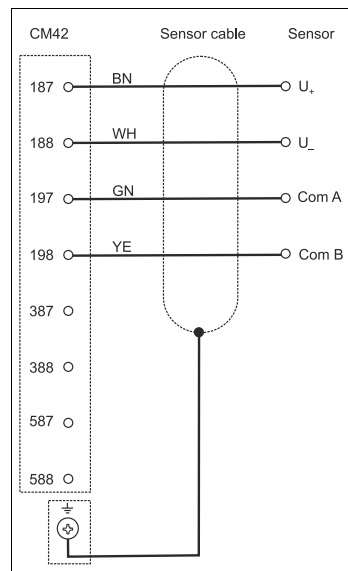

Wiring diagram

CLS50D from serial numbers J3xxxx05LI0


CLS54D from serial numbers H9xxxx05LI1

a0001078


**i** For devices with fieldbus, only new sensors (right column) may now be used.

**Sensor connection:  
analog pH/ORP sensors**

**Glass electrodes, with PAL (symmetrical)**

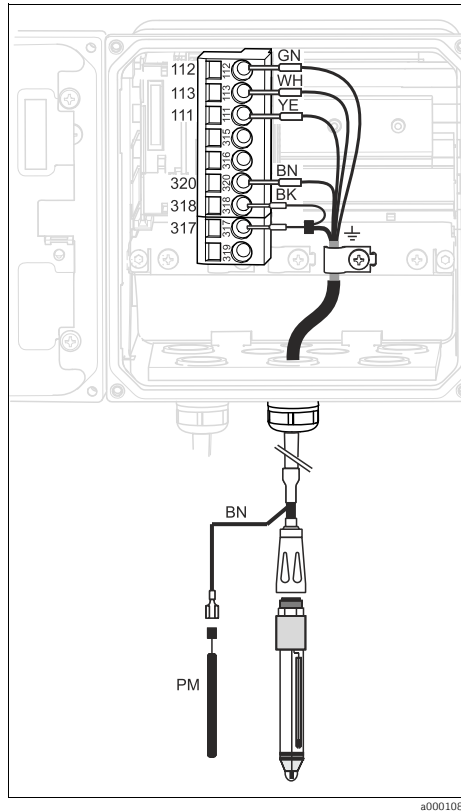


View in device (sensor module)

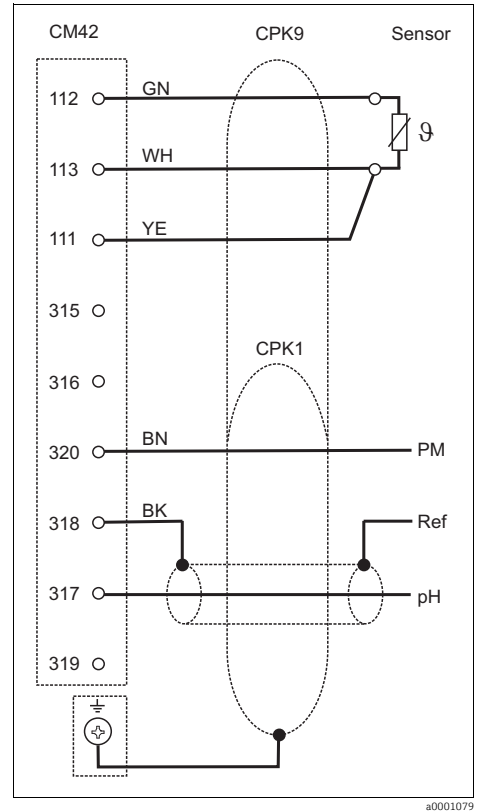


Wiring diagram

**Glass electrodes, without PAL (asymmetrical)**

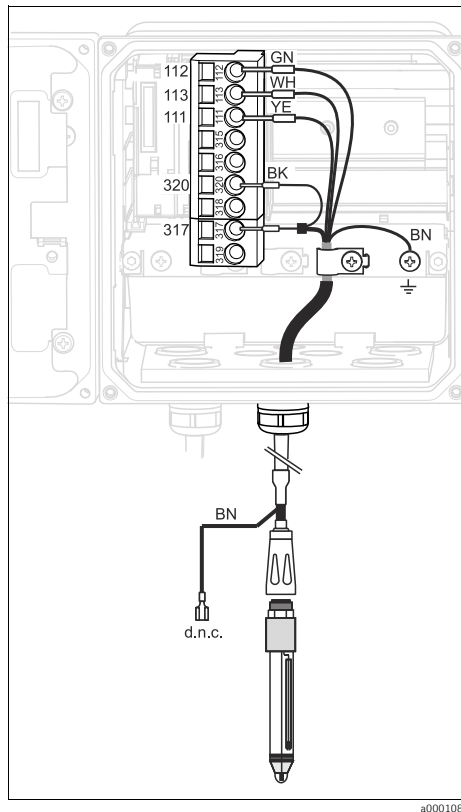


View in device (sensor module)

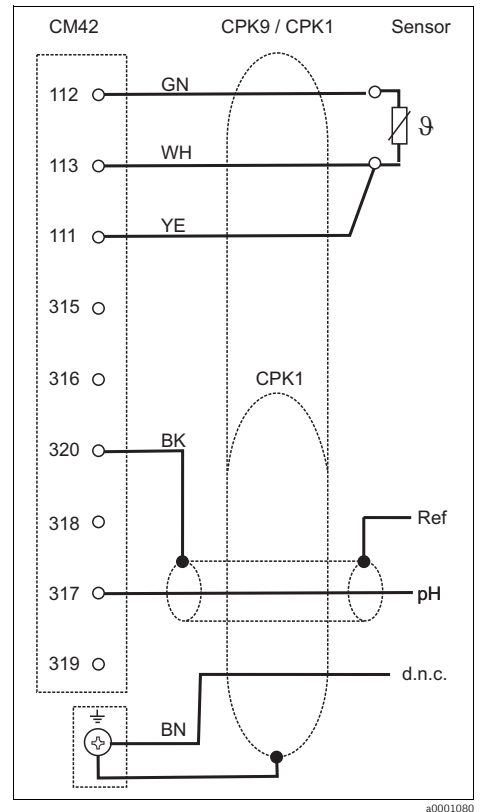


Wiring diagram

**ISFET sensors, with PAL (symmetrical)**

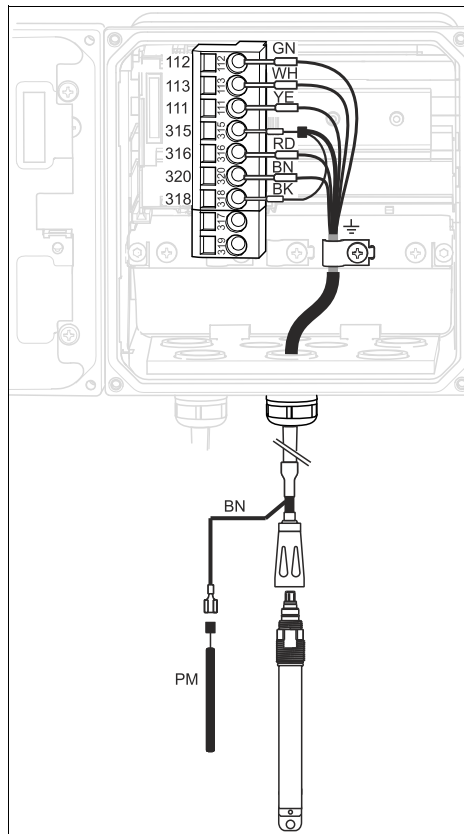

View in device (sensor module)


a0001090

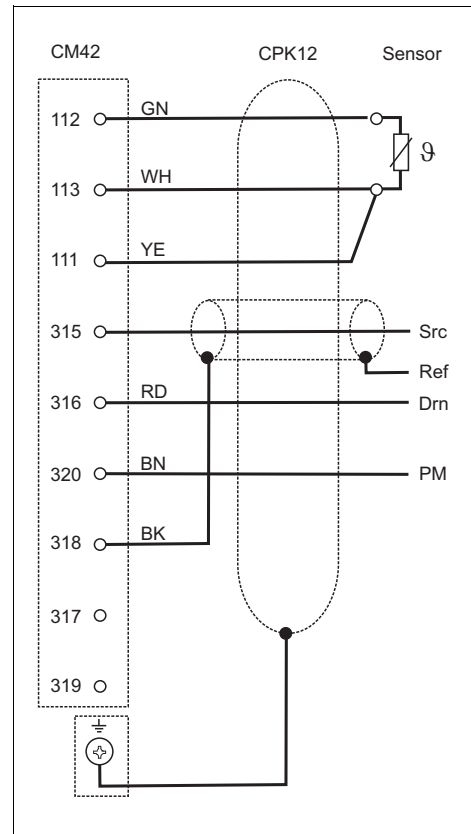

Wiring diagram


a0001076

**ISFET sensors, without PAL (asymmetrical)**

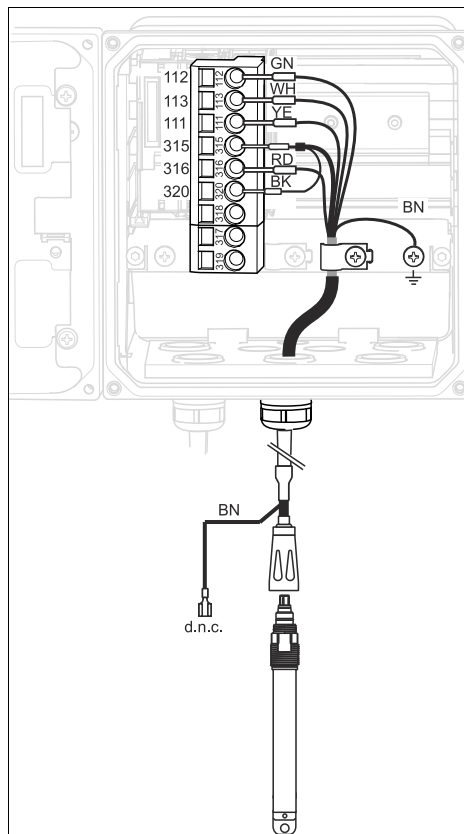

View in device (sensor module)

a0001084

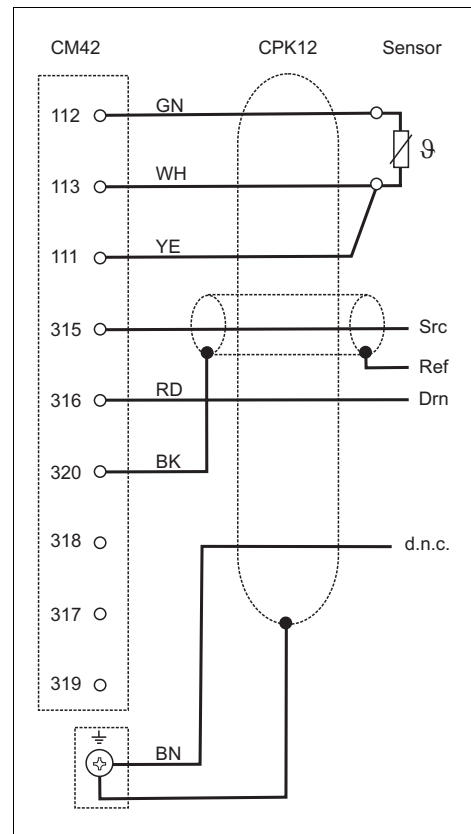


Wiring diagram

a0001077


**pH enamel electrodes**

**With PML (symmetrical)**  
 Pfaudler electrode, absolute  
 Type 03/type 04

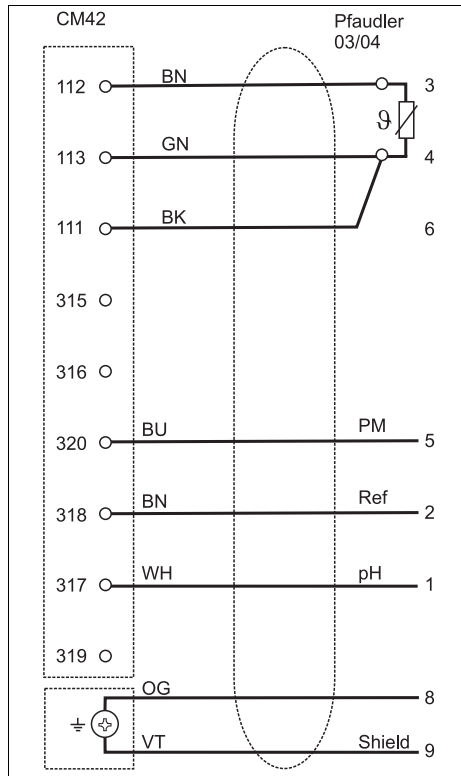


Wiring diagram

**With PML (symmetrical)**  
 Pfaudler electrode, relative  
 Type 18/type 40

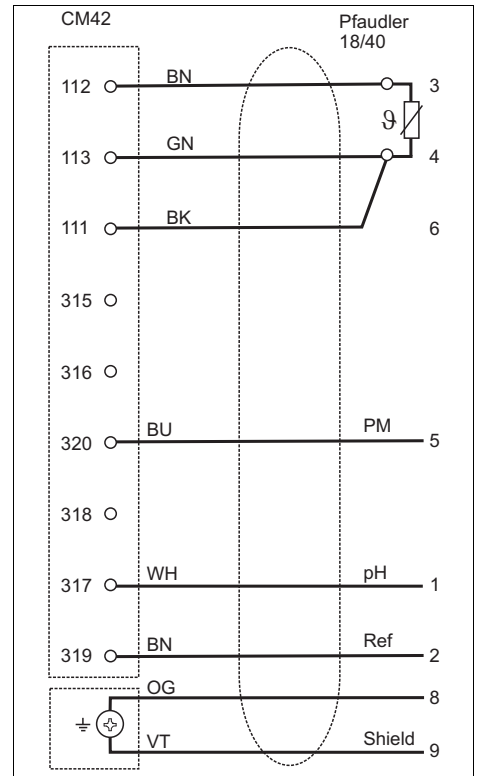


Wiring diagram

**With PML (symmetrical)**  
 pH Reiner

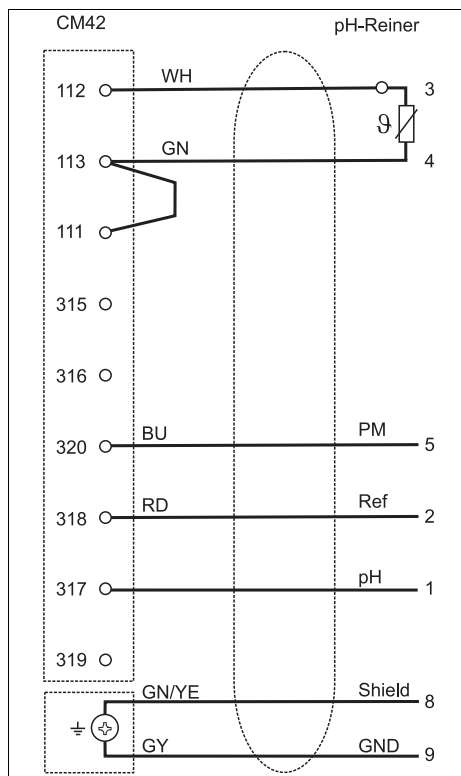


Wiring diagram

**Without PML (asymmetrical)**  
 Pfaudler electrode, absolute  
 Type 03/type 04

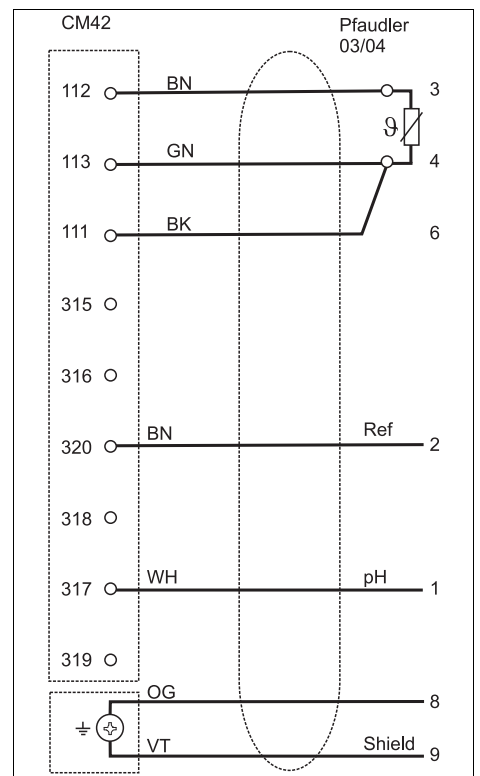


Wiring diagram

Individual electrodes (e.g. CPS64 glass or antimony), without PAL (asymmetrical)

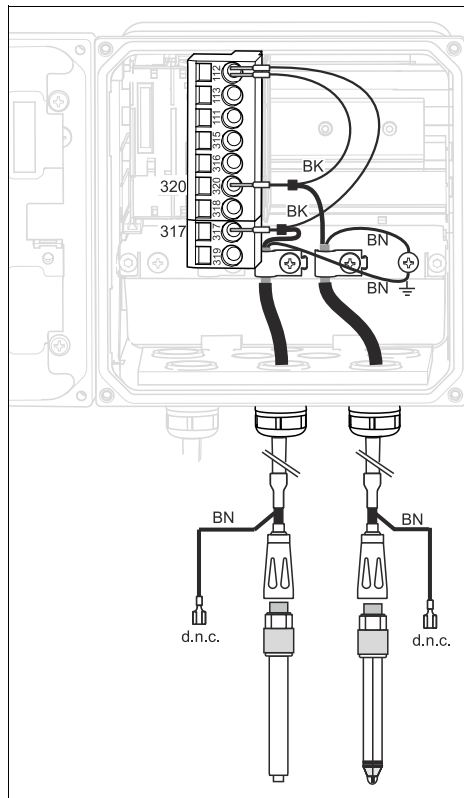


View in device (sensor module)

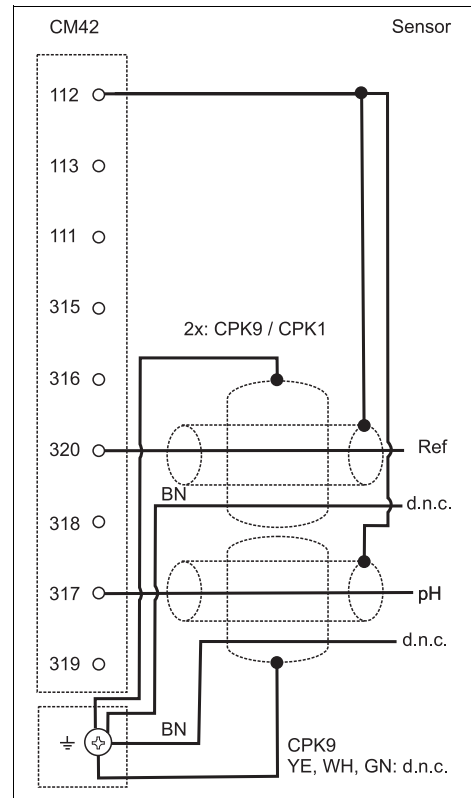

Wiring diagram

Glass electrode and ORP sensor for rH measurement

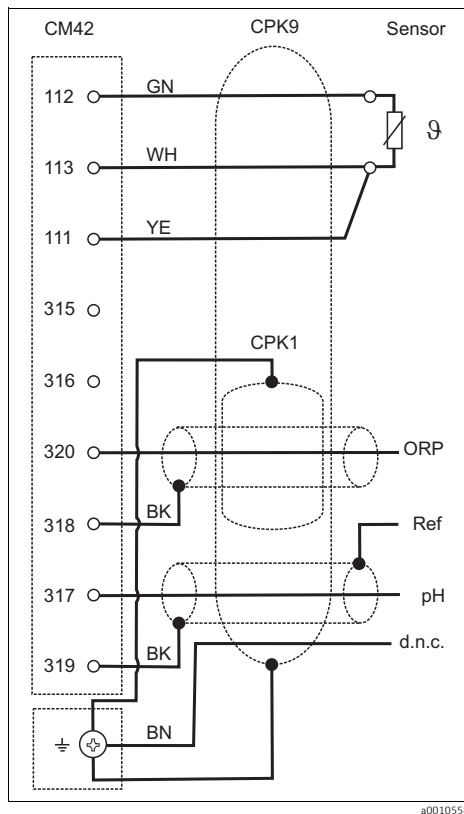


Wiring diagram

**i** For rH measurement, connect a pH combination electrode (e.g. CPS11 with sensor cable CPK9) **and** an ORP sensor (e.g. CPS12 with sensor cable CPK1).


**Sensor connection:  
analog conductivity sensors**

**Conductive sensors, two-electrode sensors**

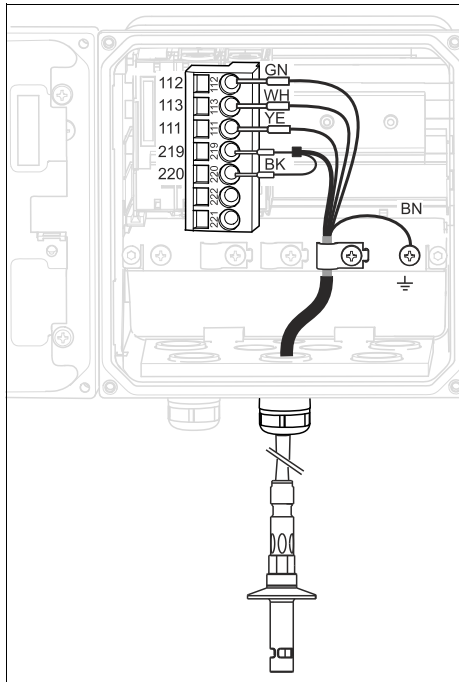

View in device (sensor module)


a0001086

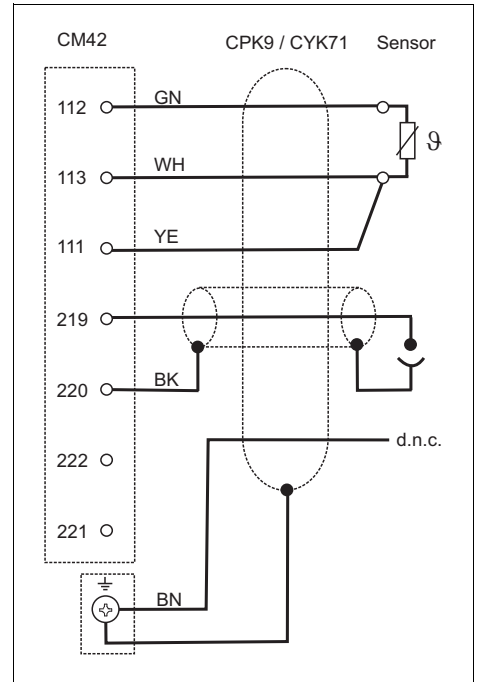

Wiring diagram


a0001083

**Conductive sensors, four-electrode sensors**

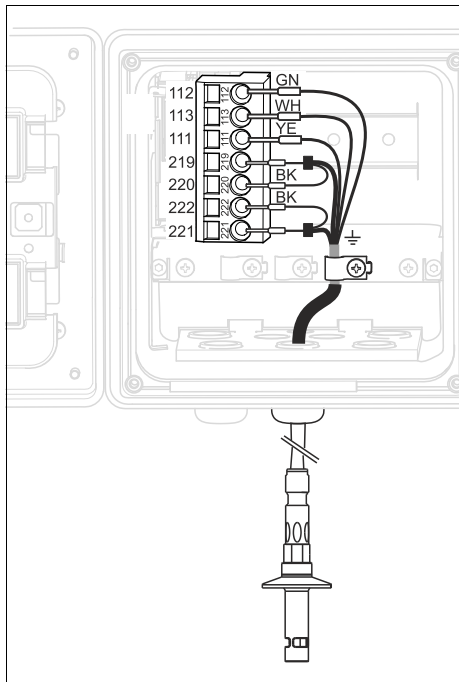

View in device (sensor module)


a0002384

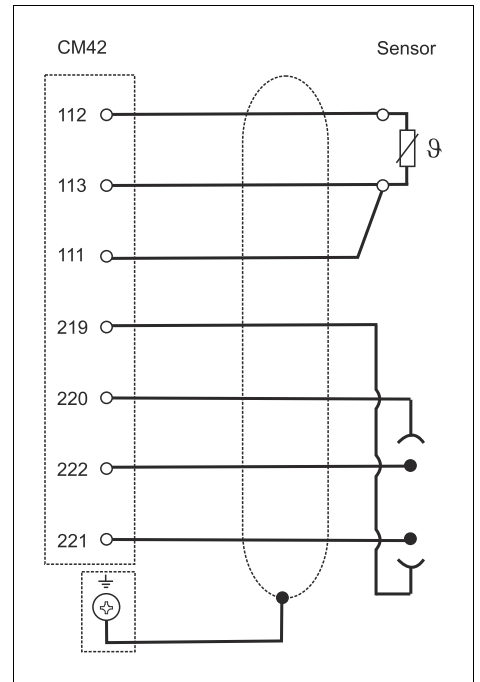

Wiring diagram

a0002371

**Inductive sensors**

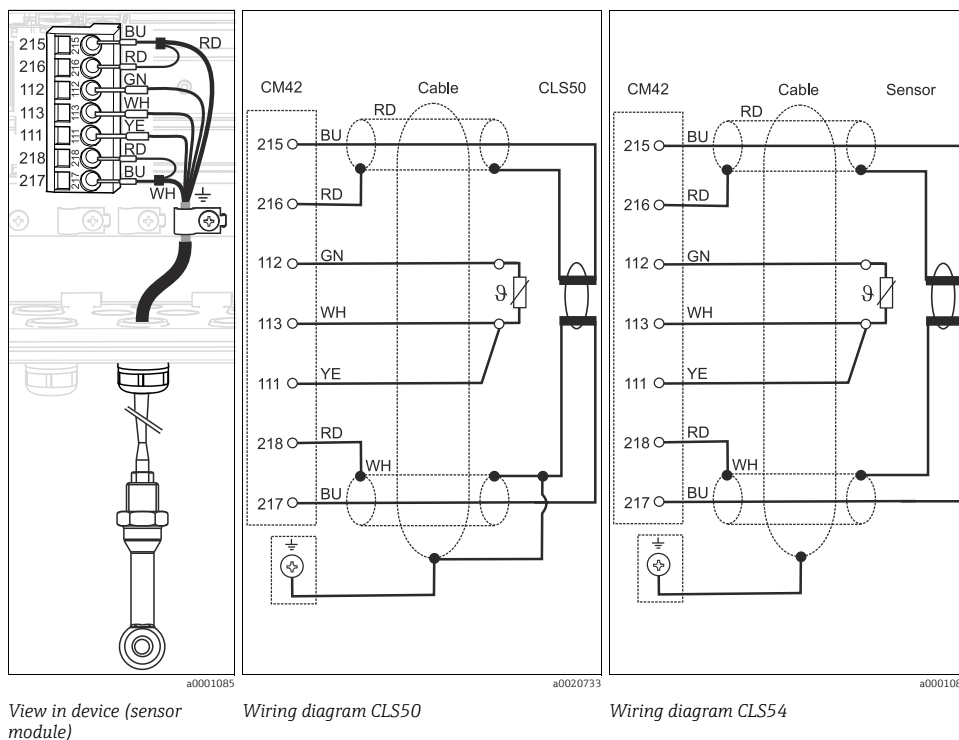

View in device (sensor module)

Wiring diagram CLS50

Wiring diagram CLS54

**Performance characteristics**

|                                     |  |       |
|-------------------------------------|--|-------|
| <b>Reference temperature</b>        | Standard 25 °C (77 °F)<br>configurable from -5 to 100 °C (23 to 212 °F) <sup>5)</sup>  |       |
| <b>Current output response time</b> | t <sub>90</sub> = max. 500 ms for an increase from 4 to 20 mA  |       |
| <b>Memosens measured error</b>      | Thanks to digital data transmission, the measured value supplied by the sensor at the sensor input is passed on accurately. Measurement accuracy depends solely on the connected sensor and the quality of its adjustment. |       |
| <b>Tolerance, current outputs</b>   | Current outputs, additional  | 25 µA |
| <b>Repeatability</b>                | --> Documentation of the connected sensor  |       |

|  |   |  |
|--|---|--|
| <b>Temperature compensation conductivity</b> | <b>Types of compensation</b>  | <b>Range</b>   |
|  | None<br>Linear<br>NaCl to IEC 746-3<br>Natural waters to IEC 7888<br>Ultrapure water NaCl<br>Ultrapure water HCl (also for NH <sub>3</sub> )<br>4 user-definable tables <sup>1)</sup> | $\alpha = 0.00$ to $20.00\% \cdot K^{-1}$<br>0 to 100 °C (32 to 212 °F)<br>0 to 35 °C (32 to 95 °F)<br>0 to 100 °C (32 to 212 °F)<br>0 to 60 °C (32 to 140 °F) |

1) with "Advanced" software package

5) with "Advanced" software package




Temperature adjustment

|                      |                           |
|----------------------|---------------------------|
| Temperature offset   | -5 to +5 °C (23 to 41 °F) |
| Temperature increase | 0.9 ... 1.1 <sup>1)</sup> |

1) with "Advanced" software package

Installation

Wall securing plate

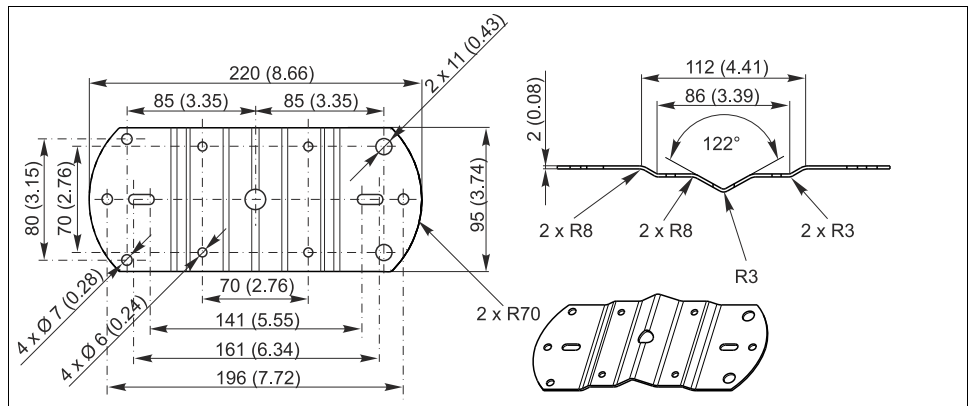

Dimensions of mounting plate in mm (inch)

Weather protection cover


**NOTICE**

**Effect of climatic conditions (rain, snow, direct sun etc.)**

Impaired operation to complete transmitter failure


- ▶ When installing outside, always use the weather protection cover (accessory).

Weather protection cover for plastic housing

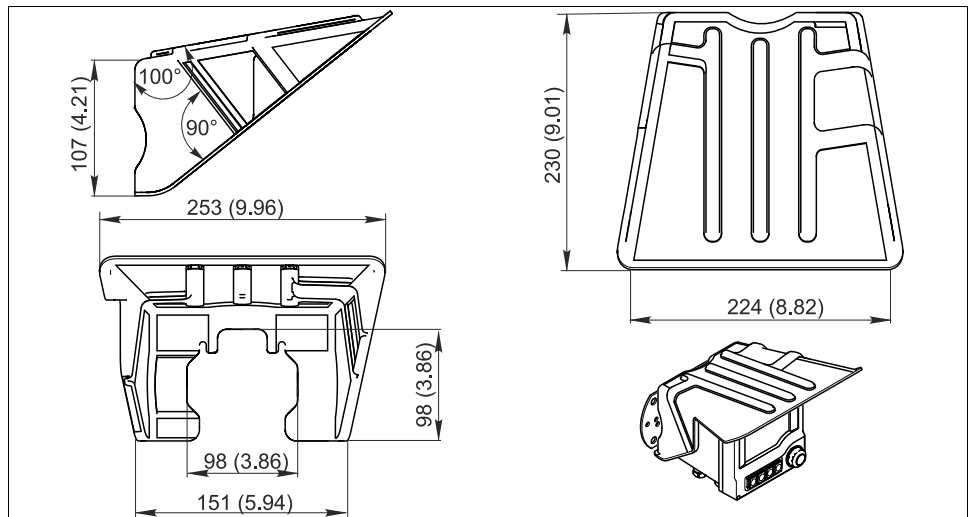

Dimensions of weather protection cover in mm (inch)

**Weather protection cover for stainless steel housing**

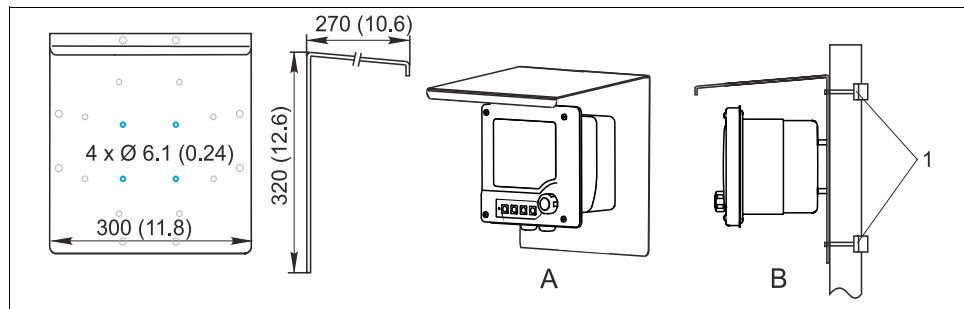


a0001676

Dimensions of weather protection cover CY101 in mm (inch)

- A Wall mounting
- B Pipe or circular post mounting
- 1 Circular post attachment (accessory)


**i** To mount the weather protection cover on pipes or circular posts, you will also require a circular post attachment, --> "Accessories" or "Installation options"

**Installation options**

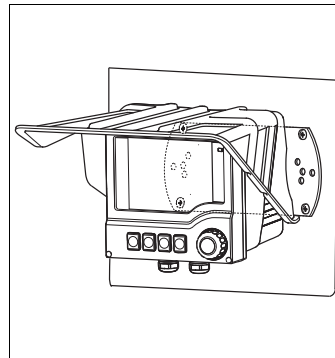


a0002166

Wall mounting  
- Weather protection cover (optional)

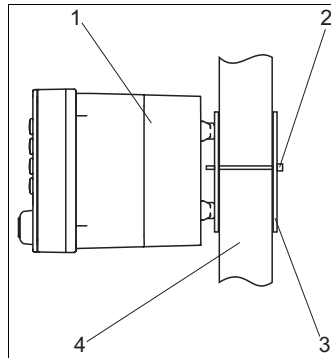



a0003092

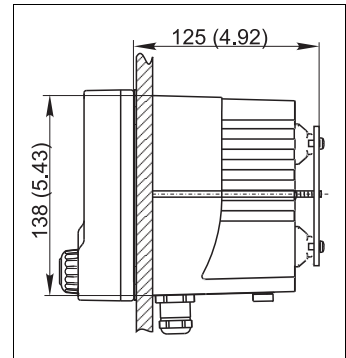Post mounting  
1 Liquiline  
2, 3 Mounting plate (1x accessory)  
4 Pipe or post (circular/square)




a0005036

Panel mounting

|   | Wall mounting                    | Pipe mounting             | Panel mounting   |
|---|----------------------------------|---------------------------|--|
| <b>Plastic housing</b>  |                                  |                           |  |
|  | without weather protection cover | Mounting plate Standard   | Mounting kit: 51518263<br>Installation kit: 51518173           |
|   | with weather protection cover    | Protection cover 51517382 | Mounting kit: 51518263<br>Protection cover 51517382            |
| <b>Stainless steel housing</b>  |                                  |                           |  |
|  | without weather protection cover | Mounting plate Standard   | Mounting kit: 51518286<br>Installation kit: 51518284           |
|   | with weather protection cover    | Protection cover CY101-A  | Protection cover CY101-A<br>Circular post attachment: 50062121 |

Installation in Ex area

CM42-\*G

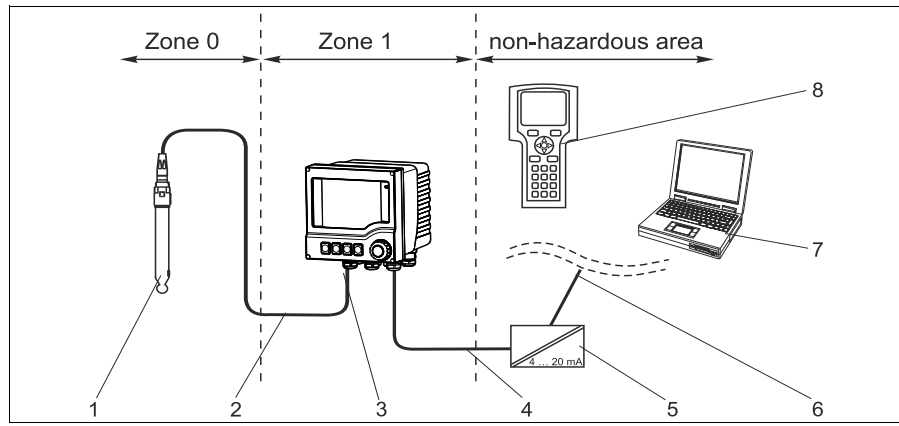


a0001312-en

Installation in Ex area

- |   |  |   |                                    |
|---|--|---|------------------------------------|
| 1 | Sensor in Ex version                         | 5 | Active barrier, e.g. Preline RN221 |
| 2 | Intrinsically safe sensor circuit Ex ia      | 6 | Signal line HART/PROFIBUS/FF       |
| 3 | Transmitter                                  | 7 | Fieldcare via PROFIBUS/FF          |
| 4 | Supply and signal circuit Ex ib (4 to 20 mA) | 8 | HART handheld terminal             |

CM42-\*V

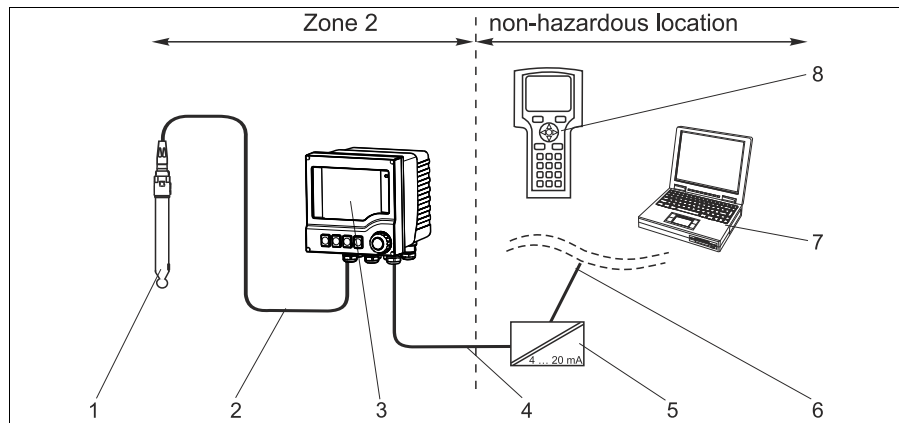


a0014574-en

Installation in Ex area

- |   |  |   |                                    |
|---|--|---|------------------------------------|
| 1 | Sensor in Ex version                         | 5 | Active barrier, e.g. Preline RN221 |
| 2 | Intrinsically safe sensor circuit Ex ic      | 6 | Signal line HART/PROFIBUS/FF       |
| 3 | Transmitter                                  | 7 | FieldCare via PROFIBUS/FF          |
| 4 | Supply and signal circuit Ex nA (4 to 20 mA) | 8 | HART handheld terminal             |


**CM42-\*P/S**

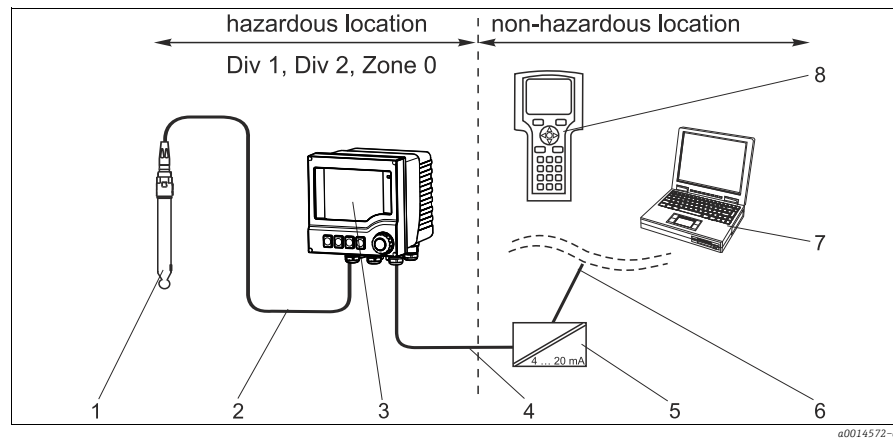

Installation in Ex area

- |   |  |   |                                    |
|---|--|---|------------------------------------|
| 1 | Sensor in Ex version                   | 5 | Active barrier, e.g. Preline RN221 |
| 2 | Intrinsically safe sensor circuit      | 6 | Signal line HART/PROFIBUS/FF       |
| 3 | Transmitter                            | 7 | FieldCare via PROFIBUS/FF          |
| 4 | Supply and signal circuit (4 to 20 mA) | 8 | HART handheld terminal             |

**CM42-\*X/Z**

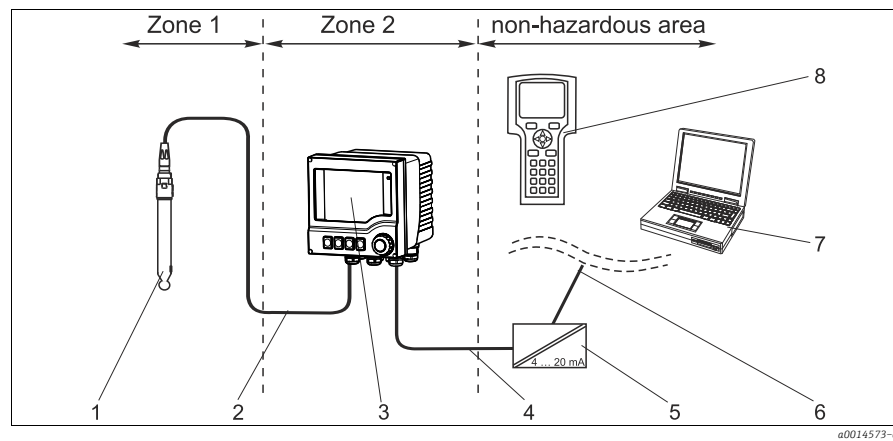

Installation in Ex area

- |   |  |   |                                    |
|---|--|---|------------------------------------|
| 1 | Sensor in Ex version                         | 5 | Active barrier, e.g. Preline RN221 |
| 2 | Intrinsically safe sensor circuit Ex ia      | 6 | Signal line HART/PROFIBUS/FF       |
| 3 | Transmitter                                  | 7 | FieldCare via PROFIBUS/FF          |
| 4 | Supply and signal circuit Ex nA (4 to 20 mA) | 8 | HART handheld terminal             |


## Environment

|                                      |  |
|--------------------------------------|--|
| <b>Ambient temperature range</b>     | <b>Non-Ex version</b><br>-30 to 70 °C (-20 to 160 °F)  |
|                                      | <b>Ex version: ATEX (1)2G &amp; 3D, ATEX 3G nA[ic] /NEPSI nA[ic], IECEx ib Gb [ia Ga], NEPSI ib[ia Ga]</b><br>-20 to 50 °C (T6)<br>-20 to 55 °C (T4) |
|                                      | <b>Ex version: ATEX 3G nA[ia], NEPSI nA[ia]</b><br>-10 to 50 °C (T6)   |
|                                      | <b>Ex version: TIIS ib</b><br>-20 to 55 °C (T4)  |
|                                      | <b>Ex version: CSA Class I, II, III, Div. 1&amp;2, FM Class I, Div 1&amp;2</b><br>-20 to 50 °C (0 to 120 °F) (T6)<br>-20 to 55 °C (0 to 130 °F) (T4) |
| <b>Storage temperature</b>           | -40 to 80 °C (-40 to 175 °F)   |
| <b>Electromagnetic compatibility</b> | Interference emission and interference immunity as per EN 61326-1: 2006, Category B (residential environments)                                       |
| <b>Degree of protection</b>          | IP66 / IP 67 / NEMA 4X   |
| <b>Relative humidity</b>             | 10 ... 95%, not condensing   |
| <b>Pollution degree</b>              | The product is suitable for pollution degree 3 as per EN 61010-1.  |

## Mechanical construction

### Dimensions


### Plastic housing

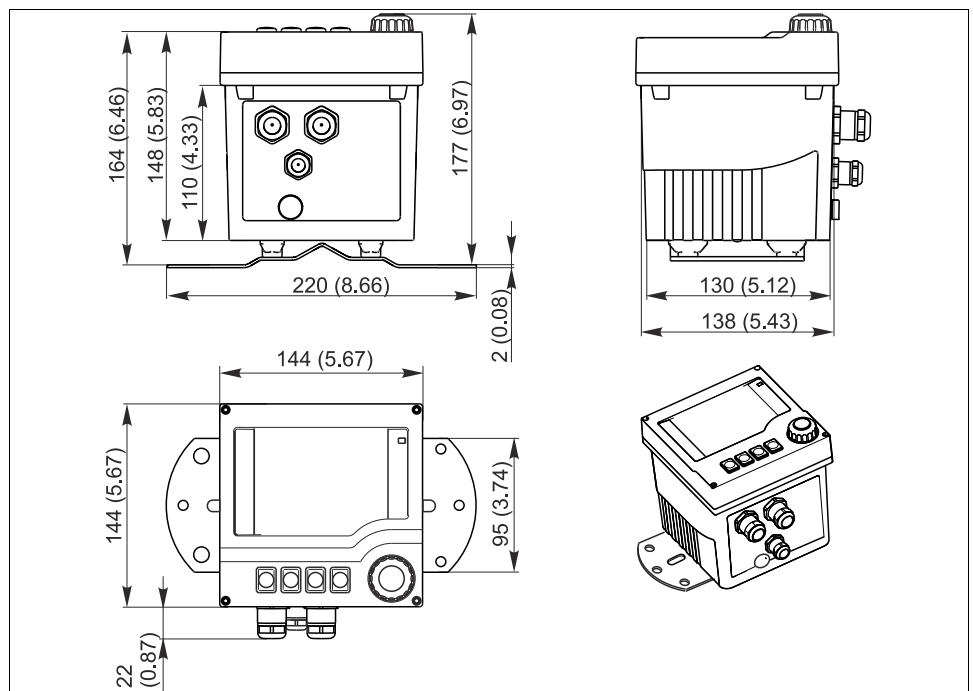

Dimensions in mm (inch)

a0011834

**Stainless steel housing**

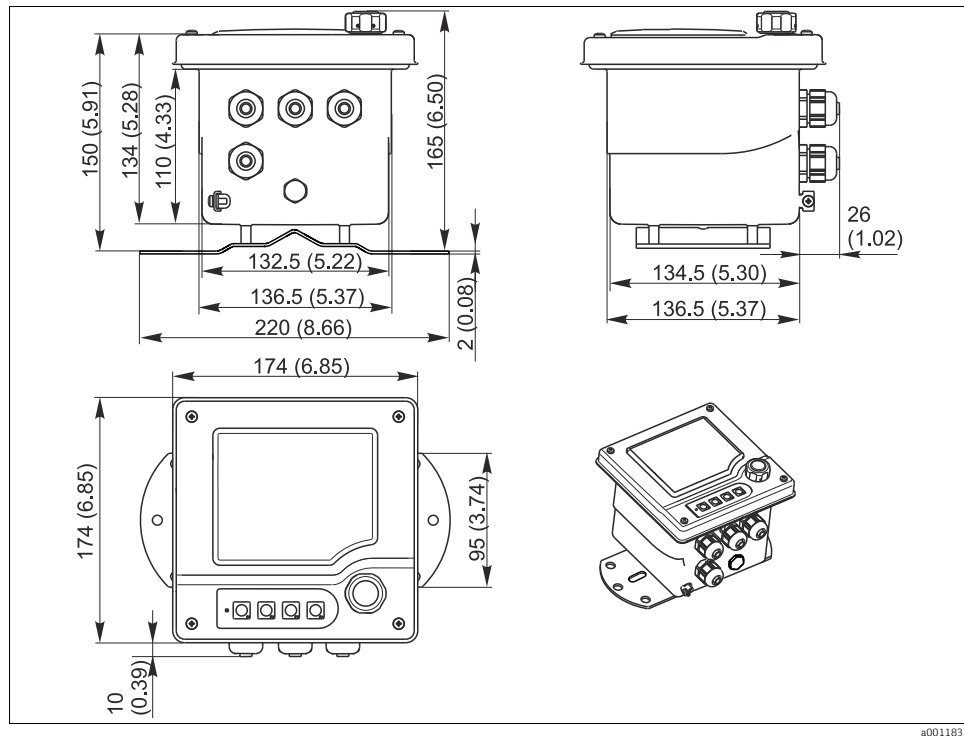

Dimensions in mm (inch)

**Weight**

**Plastic housing**

1.5 kg (3.3 lbs)

**Stainless steel housing**

2.1 kg (4.6 lbs)

**Material**

|  |   |
|--|---|
| <p><b>Plastic housing</b></p> <p>Housing</p> <p>Housing seals</p> <p><b>Stainless steel housing</b></p> <p>Housing</p> <p>Housing seals</p> <p><b>Plastic and stainless steel housing</b></p> <p>Module housing</p> <p>Soft keys</p> <p>Cable mounting rail</p> <p>Display panel</p> <p>Cable glands</p> <p>Dummy plug M16 and M20</p> | <p>PC-FR (polycarbonate, flame-retardant)</p> <p>Foamed silicone, EPDM</p> <p>Stainless steel 1.4301 (AISI 304)</p> <p>EPDM</p> <p>PC (polycarbonate)</p> <p>TPE</p> <p>Stainless steel 1.4301 (AISI 304)</p> <p>PC-FR (polycarbonate, flame-retardant)</p> <p>PA (polyamide) V0 as per UL94</p> <p>PA (polyamide) V0 as per UL94</p> |
|--|---|

## Operability

### Operation concept


The unique operating concept sets new standards:

- Fewer user errors thanks to very easy operation
- Rapid configuration using the Navigator.
- Intuitive configuration and diagnosis due to plain text display



a0001984

Navigator

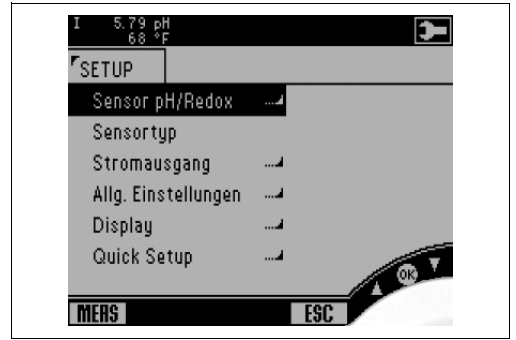

a0010473

Plain text menu


### Display characteristics

LCD display: FSTN technology (FSTN = Foil Super Twisted Nematic)

Size: 94 x 76 mm (3.7 x 3.0")

Resolution: 240 x 160 dots

### Operating elements

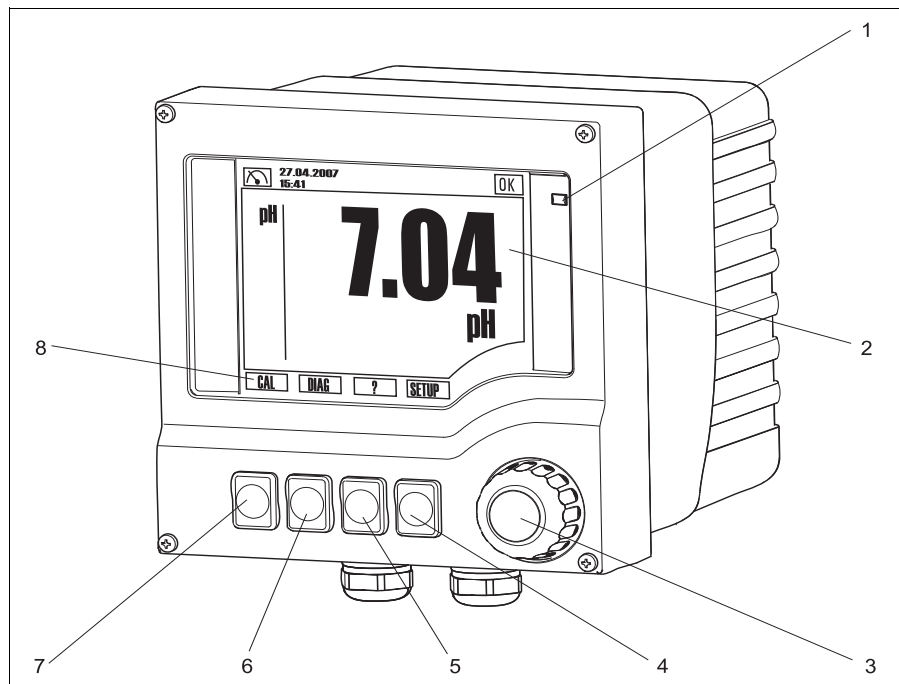

a0010480

#### Operation overview

- 1 Alarm LED
- 2 Display, current display: pH measuring mode
- 3 Navigator
- 4-7 Softkeys
- 8 Display of softkey function (menu-dependent)

---

## Ordering information

---

|                             |   |
|-----------------------------|---|
| <b>Product page</b>         | You can create a valid and complete order code on the Internet using the Configurator tool.<br>Enter the following address in the browser to launch the product page:<br><a href="http://www.endress.com/cm42">www.endress.com/cm42</a>   |
| <b>Product configurator</b> | On the right-hand side of the product page, you will find the navigation area: <ol style="list-style-type: none"> <li>1. Under "Device Support", click "Configure your selected product". <ul style="list-style-type: none"> <li>↳ The Configurator opens in a new window.</li> </ul> </li> <li>2. Configure the device according to your requirements by selecting all options. <ul style="list-style-type: none"> <li>↳ This ensures that you will receive a valid and complete order code.</li> </ul> </li> <li>3. Export the order code as a PDF or Excel file. To do so, click on the relevant button at the top of the selection window.</li> </ol> |
| <b>Scope of delivery</b>    | Depending on the version, the scope of delivery comprises:: <ul style="list-style-type: none"> <li>▪ 1 transmitter in the version ordered</li> <li>▪ 1 mounting plate incl. 4 flat head screws</li> <li>▪ 1 sheet of adhesive labels (nameplate, terminal connection diagrams)</li> <li>▪ 1 test certificate to EN 10204-3.1</li> <li>▪ 1 factory calibration certificate</li> <li>▪ Operating Instructions Part 1 and 2, BA00381C and BA00382C, in the language ordered</li> <li>▪ 1 manufacturer's certificate</li> <li>▪ Safety Manual</li> <li>▪ Maintenance Documentation SIL 2</li> </ul>   |

---


## Certificates and approvals

---

|                    |   |
|--------------------|---|
| <b>CE mark</b>     | <b>Declaration of conformity</b><br>The product meets the requirements of the harmonized European standards.<br>It therefore complies with the statutory requirements of the EC directives.<br>The manufacturer confirms successful testing of the product by affixing the <b>CE</b> symbol.  |
| <b>Ex approval</b> | Depending on the version ordered: <ul style="list-style-type: none"> <li>▪ ATEX II (1)2G Ex ib [ia Ga] IIC T4/T6 Gb / II 3 D Ex tc IIIC T85°C Dc</li> <li>▪ ATEX II (1)2G Ex ib [ia Ga] IIC T4/T6 Gb</li> <li>▪ ATEX II 3D Ex tc [ic IIC Gc] IIIC T85°C Dc</li> <li>▪ ATEX II 3G Ex nA [ic Gc] IIC T4/T6 Gc</li> <li>▪ ATEX II (2)3G Ex nA [ia Ga] IIC T6 Gc</li> <li>▪ NEPSI Ex nA [ia Ga] IIC T6 Gc</li> <li>▪ NEPSI Ex ib [ia Ga] IIC T4/T6 Gb</li> <li>▪ CSA IS NI Cl.I, II, III, Div. 1&amp;2, Grps. A-G</li> <li>▪ FM IS NI Cl.I, Div. 1&amp;2, Grps. A-D</li> <li>▪ TIIS Ex ib IIC T4</li> </ul> |



## Accessories

 The following is a list of the most important accessories available at the time this documentation was issued. For accessories not listed here, please contact your local service or sales center.

### Mounting kits

Post retainer for plastic housing

- 1 Mounting plate
- 2 Threaded rods M5x75 mm A2
- 2 Hexagonal nuts M5 A2, DIN 934
- 2 spring washers A2 DIN127, form B5 (M5)
- 2 Washers A 5.3, DIN125 A2
- Order No. 51518263

Post retainer for stainless steel housing

- 1 Mounting plate
- 2 Threaded rods M5x75 mm A2
- 2 Hexagonal nuts M5 A2, DIN 934
- 2 spring washers A2 DIN127, form B5 (M5)
- 2 Washers A 5.3, DIN125 A2
- Order No. 51518286

Panel installation kit for plastic housing for panel cutout 138x138 mm (5.43x5.43 inch)

- 1 Panel installation seal
- 2 Tensioning screws M6x150 mm
- 4 Hexagonal nuts M6, DIN934 A2
- 4 spring washers, A2 DIN127, form B6
- 4 Washers A6.4, DIN125 A2
- Order No. 51518173

Panel installation kit for stainless steel housing for panel cutout 138x138 mm (5.43x5.43 inch)

- 1 Panel installation seal
- 2 Tensioning screws M6x150 mm
- 4 Hexagonal nuts M6, DIN934 A2
- 4 spring washers, A2 DIN127, form B6
- 4 Washers A6.4, DIN125 A2
- Order No. 51518284

### Weather protection cover

Weather protection cover for plastic housing

- Order No. 51517382

Weather protection cover for stainless steel housing

- Order No. CYY101-A

### Active barrier

Active barrier RN221N

- With power supply for safe isolation of 4 to 20 mA standard signal circuits
- Technical Information TI073R/09/en

### Fieldbus accessories

Fieldbus connection socket

- FOUNDATION Fieldbus M20 7/8" connection
- Order No. 51517974

M12 connector

- Four-pole metal connector for mounting on transmitter
- For connecting to the connection box or cable jack, cable length 150 mm (5.91")
- Order No. 51502184

C-module accessories bag

- 1 capacitor for connecting the cable shielding to ground potential
- Kit documentation SD00108C
- Order No. 71003097

**Measuring cable****Memosens data cable CYK10**

- For digital sensors with Memosens technology  
pH, ORP, oxygen (amperometric), chlorine, conductivity (conductive)
- Order as per product structure (--> Online Configurator, [www.endress.com/cyk10](http://www.endress.com/cyk10))
- Technical Information TI00118C/07/EN

**Memosens data cable CYK11**

- Extension cable for digital sensors with Memosens protocol
- Order as per product structure (--> Online Configurator, [www.endress.com/cyk11](http://www.endress.com/cyk11))

**Measuring cable CPK9**

- For sensors with ESA plug-in head, for high-temperature and high-pressure applications, IP 68
- Order as per order structure
- Technical Information TI00501C/07/EN

**Special measuring cable CPK12**

- For ISFET sensors and pH/ORP glass electrodes with TOP68 plug-in head
- Order as per order structure
- Technical Information TI00118C/07/EN

**Measuring cable CYK71**

- non-terminated cable for connecting sensors and for extending sensor cables
- sold by the meter, order numbers:
  - non-Ex version, black: 50085333
  - Ex version, blue: 50085673

**Measuring cable CLK6**

- Extension cable for extending CLS50/52/54 and transmitter via VBM junction box, sold by the meter
- Order No. 71183688

**Sensors****pH/ORP glass sensors****Orbisint CPS11/CPS11D**

- pH electrode for process engineering
- Optional SIL version for connecting to SIL transmitter
- With dirt-repellent PTFE diaphragm
- Order as per product structure (--> Online Configurator, [www.endress.com/cps11](http://www.endress.com/cps11) or [www.endress.com/cps11d](http://www.endress.com/cps11d))
- Technical Information TI00028C/07/EN

**Orbisint CPS12/CPS12D**

- ORP electrode for process engineering
- Order as per product structure (--> Online Configurator, [www.endress.com/cps12](http://www.endress.com/cps12) or [www.endress.com/cps12d](http://www.endress.com/cps12d))
- With dirt-repellent PTFE diaphragm
- Technical Information TI00367C/07/EN

**Ceraliquid CPS41/CPS41D**

- pH electrode with ceramic diaphragm and KCl liquid electrolyte;
- Order as per product structure (--> Online Configurator, [www.endress.com/cps41](http://www.endress.com/cps41) or [www.endress.com/cps41d](http://www.endress.com/cps41d))
- Technical Information TI00079C/07/EN

**Ceraliquid CPS42/CPS42D**

- Redox electrode with ceramic diaphragm and KCl liquid electrolyte;
- Order as per product structure (--> Online Configurator, [www.endress.com/cps42](http://www.endress.com/cps42) or [www.endress.com/cps42d](http://www.endress.com/cps42d))
- Technical Information TI00373C/07/EN

**Ceragel CPS71/CPS71D**

- pH electrode with double-chamber reference system and integrated bridge electrolyte;
- Order as per product structure (--> Online Configurator, [www.endress.com/cps71](http://www.endress.com/cps71) or [www.endress.com/cps71d](http://www.endress.com/cps71d))
- Technical Information TI00245C/07/EN

**Ceragel CPS72/CPS72D**

- ORP electrode with double-chamber reference system and integrated bridge electrolyte;
- Order as per product structure (--> Online Configurator, [www.endress.com/cps72](http://www.endress.com/cps72) or [www.endress.com/cps72d](http://www.endress.com/cps72d))
- Technical Information TI00374C/07/EN

**Orbipore CPS91/CPS91D**

- pH electrode with open aperture diaphragm for media with high contamination potential;
- Order as per product structure (--> Online Configurator, [www.endress.com/cps91](http://www.endress.com/cps91) or [www.endress.com/cps91d](http://www.endress.com/cps91d))
- Technical Information TI00375C/07/EN

**Orbipore CPS92/CPS92D**

- ORP electrode with open aperture diaphragm for media with high contamination potential;
- Order as per product structure (--> Online Configurator, [www.endress.com/cps92](http://www.endress.com/cps92) or [www.endress.com/cps92d](http://www.endress.com/cps92d))
- Technical Information TI00435C/07/EN

**pH/ORP combined sensors****Memosens CPS16D**

- pH ORP combined sensor for process engineering, with dirt-repellent PTFE diaphragm
- With Memosens technology
- Order as per product structure (--> Online Configurator, [www.endress.com/cps16d](http://www.endress.com/cps16d))
- Technical Information TI00503C/07/EN

**Memosens CPS76D**

- pH ORP combined sensor for process engineering, hygiene and sterile applications
- With Memosens technology
- Order as per product structure (--> Online Configurator, [www.endress.com/cps76d](http://www.endress.com/cps76d))
- Technical Information TI00506C/07/EN

**Memosens CPS96D**

- pH and ORP combined sensor for chemical processes
- With poison-resistant reference with ion trap
- With Memosens technology
- Order as per product structure (--> Online Configurator, [www.endress.com/cps96d](http://www.endress.com/cps96d))
- Technical Information TI00507C/07/EN

**pH-ISFET sensors****Tophit CPS471/CPS471D**

- Sterilizable and autoclavable ISFET sensor for food and pharmaceuticals, process technology
- Water treatment and biotechnology
- Order as per product structure (--> Online Configurator, [www.endress.com/cps471](http://www.endress.com/cps471) or [www.endress.com/cps471d](http://www.endress.com/cps471d))
- Technical Information TI00283C/07/EN

**Tophit CPS441/CPS441D**

- Sterilizable ISFET sensor for media with low conductivity
- Liquid KCl electrolyte
- Order as per product structure (--> Online Configurator, [www.endress.com/cps441](http://www.endress.com/cps441) or [www.endress.com/cps441d](http://www.endress.com/cps441d))
- Technical Information TI00352C/07/EN

**Tophit CPS491/CPS491D**

- ISFET sensor with open aperture diaphragm for media with high contamination potential
- Order as per product structure (--> Online Configurator, [www.endress.com/cps491](http://www.endress.com/cps491) or [www.endress.com/cps491d](http://www.endress.com/cps491d))
- Technical Information TI00377C/07/EN

**Enamel pH electrode****Ceramax CPS341D**

- pH electrode with pH-sensitive enamel
- For the toughest requirements in terms of measurement accuracy, pressure, temperature, sterility and operating life
- Order as per product structure (--> Online Configurator, [www.endress.com/cps341d](http://www.endress.com/cps341d))
- Technical Information TI00468C/07/EN

**Inductive conductivity sensors**

## Indumax P CLS50D/CLS50

- Highly-resistant inductive conductivity sensor for standard, Ex and high-temperature applications
- With or without Memosens technology
- Order as per product structure (--> Online Configurator, [www.products.endress.com/cls50d](http://www.products.endress.com/cls50d) or .../[cls50](http://www.products.endress.com/cls50))
- Technical Information TI00182C/07/EN

## Indumax H CLS52

- Inductive conductivity sensor with fast-acting temperature sensor for applications in the food industry
- Order as per product structure (--> Online Configurator, [www.endress.com/cls52](http://www.endress.com/cls52))
- Technical Information TI00167C/07/EN

## Indumax H CLS54D

- Inductive conductivity sensor with certified, hygienic design for foodstuffs, beverages, pharmaceuticals and biotechnology
- Order as per product structure (--> Online Configurator, [www.endress.com/cls54d](http://www.endress.com/cls54d))
- Technical Information TI00508C/07/EN

## Indumax H CLS54

- Inductive conductivity sensor with certified, hygienic design for foodstuffs, beverages, pharmaceuticals and biotechnology
- Order as per product structure (--> Online Configurator, [www.endress.com/cls54](http://www.endress.com/cls54))
- Technical Information TI00400C/07/EN

**Conductive conductivity sensors**

## Condumax W CLS12

- For process temperatures up to 160 °C (320 °F) and process pressures up to 40 bar (580 psi)
- Order as per product structure (--> Online Configurator, [www.endress.com/cls12](http://www.endress.com/cls12))
- Technical Information TI00082C/07/EN

## Condumax W CLS13

- For process temperatures up to 250 °C (480 °F) and process pressures up to 40 bar (580 psi)
- Order as per product structure (--> Online Configurator, [www.endress.com/cls13](http://www.endress.com/cls13))
- Technical Information TI00083C/07/EN

## Condumax CLS15/CLS15D

- Conductive conductivity sensor for pure and ultrapure water and Ex applications
- With Memosens protocol (CLS15D) or analog (CLS15)
- Order as per product structure (--> Online Configurator, [www.endress.com/cls15d](http://www.endress.com/cls15d))
- Technical Information TI00109C/07/EN

## Condumax H CLS16/CLS16D

- Hygienic, conductive conductivity sensor for pure, ultrapure water and Ex applications
- With EHEDG and 3A approval
- Optionally available with Memosens (CLS16D)
- Order as per product structure (--> Online Configurator, [www.endress.com/cls16d](http://www.endress.com/cls16d))
- Technical Information TI00227C/07/EN

## Condumax W CLS19

- Inexpensive, conductive conductivity sensor for pure and ultrapure water applications;
- Order as per product structure (--> Online Configurator, [www.endress.com/cls19](http://www.endress.com/cls19))
- Technical Information TI00110C/07/EN

## Condumax W CLS21/CLS21D

- Two-electrode sensor in version with plug-in head and fixed cable
- Optionally available with Memosens (CLS21D)
- Order as per product structure (--> Online Configurator, [www.endress.com/cls21d](http://www.endress.com/cls21d))
- Technical Information TI00085C/07/EN

**Amperometric oxygen sensors**

Oxymax COS22D

- Sterilizable sensor for dissolved oxygen
- Order as per product structure (--> Online Configurator, [www.endress.com/cos22d](http://www.endress.com/cos22d))
- Technical Information TI446C/07/EN

Oxymax COS51D

- Amperometric sensor for dissolved oxygen, with Memosens technology
- Order as per product structure (--> Online Configurator, [www.endress.com/cos51d](http://www.endress.com/cos51d))
- Technical Information TI00413C/07/EN

---

**Software update and upgrade** CY42 DAT module

- Extended functionality, update and memory module
- Ordering as per order structure

| Version |  |
|---------|--|
| C1      | CopyDAT, for saving the configuration and transferring it to other devices |
| F1      | FunctionDAT for extending the function to 2 current outputs                |
| F2      | FunctionDAT for extending the function to advanced software                |
| S1      | SystemDAT, for software update, language catalog extension                 |
| CY42-   | Complete order code  |

[www.addresses.endress.com](http://www.addresses.endress.com)

---